

QUADERA HTML Help

Table Of Contents

QUADERA® Help	1
Program version 4.40, June 2011	1
License Agreement.....	3
I Preliminary Remarks.....	3
II Agreement.....	3
1. Object of the Agreement.....	3
2. License Fees	3
3. Copyright	4
4. User Rights	4
5. Warranty and Liability.....	4
6. Additional Software	5
7. Changes and Additions to the Agreement	5
8. Governing Law.....	5
9. Exclusive Validity of this Agreement	5
Copyrights	7
Cross-References from Manuals	9
Migrating from Quadstar to QUADERA.....	11
Migrating from Quadstar to QUADERA®	11
Overview and Differences in the Used Terminology	12
Overview and Differences in the Available Functions.....	13
QUADERA	15
Introduction	15
Product Description.....	15
Product Description	15
Main Features	16
Scope of Delivery.....	17

QUADERA HTML Help	
System Requirements	19
Getting Help	20
Calling Help	20
Changing the Display of a Help Topic	21
Printing a Help Topic	22
Further Information.....	23
Reporting Errors	24
Installing and Uninstalling QUADERA	25
Installation Program SETUP.....	25
Installing.....	26
Setting Up	27
Adjusting the Device Settings.....	28
Version Number	32
Updating	33
Uninstalling	34
Operating Concept.....	35
Basics for Operation.....	35
Operating Elements	37
User Interface	37
Screen Elements.....	38
Mouse Actions	40
Keyboard Shortcuts.....	41
Customizing the Keyboard Shortcuts	42
User Interface.....	44
Title Bar	44
Menu Bar.....	45
Options	47

Table Of Contents

Toolbox	48
Measurement Project Window	53
Recipe Selection	54
Working Area	55
Working Area Selection	56
Device Status View	57
All Device Status View	58
Event View	59
Context Menus	60
Capturing Screenshots of the User Interface	71
Getting Started	72
Starting QUADERA®	72
Start Page	73
Example of a Measurement	74
Introduction	74
Course of a Measurement - Scan	75
Course of a Measurement - MID	76
Chart Display	77
Data Navigator	78
Data Navigator	78
Data Navigator and Zooming	80
Data Navigator in Scan Measurements	81
Data Navigator in MID/MCD Measurements	82
Exiting QUADERA®	83
Opening and Managing Measurement Data	84
Opening an Existing Measurement Project	84
Recently Used Files	85

QUADERA HTML Help	
Exporting a Measurement Project.....	86
Closing a Measurement Project.....	87
Changing a File Location.....	88
Changing the Display of Measurement Projects.....	89
Adjusting the Section.....	89
Zooming in Charts.....	90
Selecting Curve Colors in Charts.....	91
Defining the Line Thickness in Charts.....	92
Splitting Up the Working Area.....	93
Deleting a Section.....	94
Creating a New Working Area.....	95
Deleting a Working Area.....	96
Freezing the Display.....	97
Managing and Arranging Windows.....	98
Displaying Windows.....	98
Showing and Hiding Docker Windows.....	100
Calling Device Specific Functions.....	101
Configuring the Device Connection.....	101
Starting and Stopping the Measurement.....	102
Disconnecting From the Device.....	103
Connecting With the Device.....	104
Simulation Mode.....	105
Calibration.....	106
Calibration Projects.....	106
Tuning the Ion Source.....	107
Tuning the Ion Source.....	107
Optimizing the Ion Source.....	108

Table Of Contents

Ion Source Parameters	110
Crossbeam Ion Source.....	114
Grid Ion Source	115
SPM Ion Source	116
Open High Sensitivity Ion Source	117
Gastight High Sensitivity Ion Source	118
Tuning the Mass Scale.....	121
Calibrating the Mass Scale	121
Coarse Tuning of the Mass Scale	123
Fine Tuning of the Mass Scale.....	125
Parameters for Coarse Tuning.....	127
Parameters for Fine Tuning	129
Offset	131
Offset.....	131
Determining the Offset	132
Offset Parameters	134
Tuning the RF Generator.....	136
Tuning the RF Generator	136
Minimizing the Tuning Voltage (QMG220)	137
Minimizing the Tuning Voltage (QMG700)	139
Background Determination.....	140
Background Determination	140
Measuring the Background	141
Background Library	143
Gas Specific Calibration	146
Gas Specific Calibration	146
Determining the GSC Factors.....	147

QUADERA HTML Help	
GSC Matrix Editor	149
GSC Result View	152
MCD Calibration Factor Library	154
Enabling Partial Pressure	156
Determining the Sensitivity	156
Required Process to Enable Partial Pressure	157
Measurements using QUADERA	158
Measurement Projects and Measurement Project Templates	158
Scan Measurement Projects	159
MID Measurement Projects	160
MCD Measurement Projects	161
Total Pressure Measurement	163
Creating Measurement Project Templates	164
Recipes	165
Recipes	165
Recipe Editor	167
Recipe Parameters: Scan	169
Recipe Parameters: MID	174
Recipe Parameters: MCD	178
Recipe Parameters: Total Pressure	179
Trip Function ABS	181
Trip Function HYST	183
Processing Measurement Data	184
Minimum	184
Average	185
Maximum	186
Absolute Standard Deviation	187

Table Of Contents

Automating Tasks.....	188
Triggered Run Add-in	188
Scripting	191
Scripting.....	191
Scripting Directory Structure	192
Copying Add-ins	193
Deleting Add-ins	194
Using Macros	195
Creating Add-ins and Macros	195
Activating Add-ins.....	196
Running Macros	197
Editing Add-ins and Macros	198
Calling Up the VSTA Editor	199
Calling Up the VSTA Help	200
Spectra Library	201
Spectra Library	201
Operating the Input/Output Module	202
Creating IO Characteristics	203
Creating Input/Output Characteristics.....	203
Warning and Error Messages.....	205
List of Events	205
Warning Messages for the QMG220	206
Warning Message QMG220.W001	206
Warning Message QMG220.W002	207
Warning Message QMG220.W003	208
Error Messages for the QMG220.....	209
Error Message QMG220.E001	209

QUADERA HTML Help

Error Message QMG220.E002	210
Error Message QMG220.E003	211
Error Message QMG220.E004	212
Error Message QMG220.E005	213
Error Message QMG220.E009	214
Error Message QMG220.E039	215
Scripting in QUADERA.....	217
Glossary	219
Index	225

QUADERA® Help

Program version 4.40, June 2011

Welcome to QUADERA®, the software for controlling the mass spectrometers QMG220 and QMG700. QUADERA® is a Windows application based on Microsoft's .NET framework and other contemporary technologies. The user interface is state of the art and provides access to settings and data.



- Copyrights: Copyrights and trademarks,
- License agreement: License agreement for the QUADERA® software,
- Resources to access the online Help: The online Help contains all the information required for operating QUADERA®.

Please read the "Setting Up" section to easily configure QUADERA® and the devices.

NOTE:

Read the QUADERA® Release Notes. They list new features, bugfixes, known problems and limitations of QUADERA®. In addition, the Release Notes give important information on installing and configuring QUADERA®, on the operating system, and on the network settings.

Opening the Release Notes:

After installing QUADERA® with the default settings, proceed as follows to open the Release Notes:

- Via the Windows start menu: Program Files > QUADERA > Readme
- Open the file "Readme.html" in the directory for programs and settings.

License Agreement

Please be sure to read the conditions of this Software License Agreement.

Please direct any inquiries in writing to the following address:

USA:

INFICON Inc.
Two Technology Place
E. Syracuse NY 13057
USA

Europe and Asia:

INFICON Aktiengesellschaft
Abteilung KA
LI-9496 Balzers
Liechtenstein

I Preliminary Remarks

1. LICENSEE has purchased an equipment and/or a component from INFICON hereafter referred to as HARDWARE.
2. The SOFTWARE allows the HARDWARE to be computer controlled.
3. This contract defines the conditions under which INFICON grants the LICENSEE the right to use the SOFTWARE required for computer control of the HARDWARE.

II Agreement

1. Object of the Agreement

The SOFTWARE (program and documentation) supplied with the HARDWARE remains the property of INFICON. INFICON grants the LICENSEE non-transferable and non-exclusive rights to the use of this SOFTWARE according to the conditions given herein for an unlimited period of time but only for the HARDWARE described under Section I of this agreement

2. License Fees

The license fees for the use of the SOFTWARE under discussion in this agreement are contained in the basic price of the HARDWARE. If this SOFTWARE is supplied separately, the license fees are included in the price of the SOFTWARE.

Upon payment of the basic price, the LICENSEE is granted the right to the use of this SOFTWARE for an unlimited period of time on the HARDWARE according to the following conditions.

No counseling, introductory support, training or maintenance is included in the license fee. INFICON will only offer these services on the basis of a separate, written agreement according to the conditions in force at INFICON at that particular point in time. However, INFICON is not obligated to enter into such an agreement.

3. Copyright

INFICON has the exclusive copyright on the SOFTWARE (including the source code) under discussion in this agreement. The contract partners agree that the licensed SOFTWARE may only be used within the framework of the permission outlined in this agreement. Any other use not expressly stated in the agreement is a breach of both, the copyright and the agreement and will lead to an immediate termination of the license by INFICON with INFICON being entitled to full compensation from the LICENSEE.

The LICENSEE recognizes that the codes for the SOFTWARE are a INFICON trade secret. Any use of these codes by the LICENSEE not expressly permitted in the agreement constitutes a disclosure of this trade secret making the LICENSEE fully responsible to INFICON for damages in the declared amount of the investment and development costs for the SOFTWARE. INFICON rights as declared in Section II, Paragraph 1 also apply in this case.

The LICENSEE is obligated to undertake any and all measures required to prevent his employees from causing any of the above described breaches of contract, either during or after the period of their employment in the LICENSEE's company.

4. User Rights

Each licensed SOFTWARE under discussion in this contract has been developed by INFICON for use on the previously defined HARDWARE, its peripherals and its operating system. The conditions of use required by INFICON are specified in this agreement and in the accompanying SOFTWARE description.

The LICENSEE may make as many copies of the SOFTWARE description as needed. However, all descriptions, documentation, and one backup copy of the software remain the property of INFICON.

The rights granted in this license are not transferable.

5. Warranty and Liability

5.1 Scope of the Warranty

INFICON warrants that the SOFTWARE under discussion in this agreement will function according to the SOFTWARE specification laid down in the agreement and the conditions of use specified.

Both parties recognize that software errors can occur even when extreme care is taken.

5.2 Warranty Claims by the LICENSEE

If the object of the agreement does not meet the guaranteed specifications given with it, the LICENSEE only has the right to a correction by INFICON, and this only within the period of the warranty for the HARDWARE. If the SOFTWARE is supplied separately from the HARDWARE, the warranty time shall be 90 days from the date of delivery.

INFICON excludes any right to warranty service and liability claims if the LICENSEE or any third party makes any modification in the license product and/or the HARDWARE for which it was intended.

Any further warranty claims are expressly excluded. This exclusion includes in particular any liability for damage to the HARDWARE and/or SOFTWARE itself as well as any damage that may occur as a result of the use of this SOFTWARE.

6. Additional Software

INFICON will supply additional SOFTWARE at the cost of an additional license fee.

The conditions of this contract as described above also apply to any additionally supplied SOFTWARE.

7. Changes and Additions to the Agreement

Only written changes and additions are binding.

8. Governing Law

This agreement is subject to US and Swiss Law.

9. Exclusive Validity of this Agreement

The LICENSEE states that he has read this agreement and understands its contents. In opening the sleeve the LICENSEE indicates that he accepts this agreement as the only valid agreement between the two parties concerning the SOFTWARE under discussion therein. Any earlier oral or written agreements are nullified by this agreement. Changes must be made in writing.

QUADERA HTML Help

*INFICON
Two Technology Place
E. Syracuse NY USA
Tel +1 315 434 1100
Fax +1 315 437 3803*

reachus@inficon.com

*INFICON
LI-9496 Balzers
Furstentum Liechtenstein
Tel +423 / 388 3111
Fax +423 / 388 3700*

reach.liechtenstein@inficon.com

www.inficon.com

Copyrights

COPYRIGHTS

Copyright © 2004 - 2011 INFICON All rights reserved.

Specifications are subject to change without notice.

No part of this software and the accompanying material may be reproduced in any way nor may it be manipulated with electronic systems, duplicated or distributed without written permission from INFICON. Offenses against these regulations will result in compensation claims.

The original software delivered may not be used for purposes other than those intended nor is it permitted to make copies of the software. In particular, it is strictly forbidden to give copies of the software to other people.

The use of trade names, brand names, trademarks, etc. in this document does not entitle third parties to consider these names to be unprotected and to use them freely. This is in accordance with the meaning of the laws and acts covering brand names and trademarks.

TRADEMARKS

QUADERA® is a registered trademark of INFICON.

Microsoft® Visual Studio® Tools for Applications (VSTA) is a registered trademark of Microsoft Corp.

Cross-References from Manuals

In this topic you find cross-references from manuals that refer to the QUADERA® Online-Help. Click on the corresponding link below to display the required topic:

Cross-references from the "PrismaPlus" manual

- Cross-reference #001: System configuration
- Cross-reference #002: Commissioning
- Cross-reference #003: Measuring mode
- Cross-reference #004: EXTERNAL PROTECTION
- Cross-reference #005: Using the analog and digital interfaces
- Cross-reference #006: Optimizing the ion source sensitivity
- Cross-reference #007: Tuning the RF generator

Migrating from Quadstar to QUADERA

Migrating from Quadstar to QUADERA®

Quadstar is an application software for the QMS 422/421 and QMS 200 Prisma™ quadrupole mass spectrometers. QUADERA® and Quadstar share some basic capabilities. However, they sometimes differ in the used terminology, and especially in the functionality and the tools. Once you know these differences you will be able to migrate to QUADERA® easily.

Overview of the differences in the used terminology

Overview of the differences in the available tools and functions

Overview and Differences in the Used Terminology

The terms and concepts of Quadstar and QUADERA® differ in some ways. Many terms have a similar meaning, but they are named differently. The table below contains the terms used in Quadstar and the equivalent terms used in QUADERA®.

Quadstar term	QUADERA® term
Channel	Measurement task
Channel parameter editor	Recipe editor
Mass spectrometer	Device
Measurement	Measurement project
Measurement parameter file	Measurement project template

Overview and Differences in the Available Functions

Quadstar comprises a package of several main programs (measurement program, display program, analysis program, etc.). These programs are called up and closed individually as the need arises. In QUADERA®, on the other hand, the entire functionality is always available. It is no longer necessary to call up or close individual components. QUADERA® allows you to display several measurement projects at a time and also to display different views of one measurement project.

The following table lists several functions and shows how to call them up in Quadstar and in QUADERA®.

Notation: xxx > yyy > zzz means "In the main menu, select the item xxx. In the following submenu, select the item yyy. Then select the item zzz".

Function	Quadstar	QUADERA®
Select the simulation mode	"Parset" program: Setup > General > Simulation Mode > Intern	Device > Communication Settings... > Simulator
System information	For each main program: File > About	Help > About...
Establish a connection to the device	For each main program: Comm > Connect	Device > Connect
Open a measurement project template for Scan	Via the file manager in the "Measure" program: Scan > Analog	Via the Start page
Open a measurement project template for MID	Via the file manager in the "Measure" program: MID > Versus Time	Via the Start page
Start/stop a Scan measurement	Via the file manager in the "Measure" program: Scan > Analog > Operation > Go/Halt	Device > Run
Start/stop a MID measurement	Via the file manager in the "Measure" program: MID > Versus Time	Device > Run

QUADERA HTML Help

	> Operation > Go/Halt	
Save measuring data	Manually in the file manager: File > Save Cycle Data	Automatically
Open an existing measurement project (Scan measurement)	"Dispsav" program: Scan > Analog Data	File > Open
Open an existing measurement project (MID measurement)	"Dispsav" program: Process > Cycles	File > Open
Edit measurement parameters	Via the file manager and the channel parameter editor in the "Parset" program	Directly in the corresponding working area of the opened measurement project (Recipe Editor)
Automate measurements and analyses	Via the sequencer (command interpreter with a specific syntax) in the "Parset" program	In parts implemented via the VBA editor and the use of macros
User access	Via the "Accessc" administration program directly in Quadstar	Handled by the operating system of the PC on which QUADERA® has been installed

QUADERA

Introduction

Product Description

Product Description

QUADERA® is a powerful operation and analysis software for the following quadrupole mass spectrometers:

- QMG220
- QMG700

QUADERA® allows you to perform a qualitative and quantitative analysis.

QUADERA® simplifies the operation of the mass spectrometer, improves the reproducibility of the results, and allows you to store all relevant parameters and data. In addition, it also checks the consistency of specific parameters and issues a warning in the case of an error.

QUADERA® allows you to save and to document measuring data, to reload these data and to display the reloaded data in various ways (table, bar graph, trend etc.).

Main Features

- Easy operation via graphical user interface
- Powerful measuring programs for qualitative and quantitative analysis
- Analysis of measuring data while a measurement is running
- Display of multiple measurement tasks in a table, as a bar graph, or as a trend
- Measurements can be documented
- Service functions
- Online parametrization of the mass spectrometer
- Automatic electrometer range switching

Scope of Delivery

Software

- License agreement and license key.
- CD-ROM with QUADERA®. The supplied installation program will create the required folders and copy various files into these folders.
- Measurement project templates are supplied for all types of measurement.

Directories created during installation under Windows XP with the default settings

- Programs and settings: "C:\Program Files\QUADERA"
- Example files: "C:\Documents and Settings\[User]\My Documents\My QUADERA\Data"
- Measurement project templates: "C:\Program Files\QUADERA\[QMG]"
- Tool programs: "C:\Program Files\QUADERA\Tools"
- Simulator: "C:\Program Files\[QMG]Sim"
- Files created by the user: "C:\Documents and Settings\[User]\My Documents\My QUADERA\Data"
- Computer specific settings: "C:\Documents and Settings\All Users\Application Data\INFICON\QUADERA\[Version]"
- User specific settings: "C:\Documents and Settings\[User]\Application Data\INFICON\QUADERA\[Version]"
- Scripting: "C:\Documents and Settings\[User]\My Documents\My QUADERA\Scripting"

Notes:

[User] represents your registered profile,
[Version] indicates the currently installed version of QUADERA®,
[QMG] specifies the mass spectrometer, i.e. QMG220, QMG700.

Directories created during installation under Windows Vista with the default settings

- Programs and settings: "C:\Program Files\QUADERA"
- Example files: "C:\Users\[User]\Documents\My QUADERA\Data"
- Measurement project templates: "C:\Program Files\QUADERA\[QMG]"
- Tool programs: "C:\Program Files\QUADERA\Tools"
- Simulator: "C:\Program Files\QUADERA\[QMG]Sim"
- Files created by the user: "C:\Users\[User]\Documents\My QUADERA\Data"
- Computer specific settings: "C:\Users\All Users\QUADERA\[Version]"

QUADERA HTML Help

- User specific settings:
"C:\Users\[User]\AppData\Roaming\QUADERA\[Version]"
- Scripting: "C:\Users\[User]\Documents\My QUADERA\Scripting"

Notes:

[User] represents your registered profile,
[Version] indicates the currently installed version of QUADERA®,
[QMG] specifies the mass spectrometer, i.e. QMG220, QMG700.

Cables and Accessories

- Ethernet cable with crossed wires for direct connection of the mass spectrometer to a PC
- Normal Ethernet cable for direct connection of the mass spectrometer to a network

System Requirements

In order to install the QUADERA® software on a PC, the following minimum requirements for hardware and software must be met:

Hardware for operating system Windows XP

- Processor: Intel P3 1.5 Ghz (or other equivalent processors), recommended P4 3 GHz
- Main memory: 512 MB, recommended 1 GB
- Free space on the harddisk: 100 MB to install the program, additional space for the measurement data
- Graphics card: Resolution 1024 x 768 pixels or higher, at least 256 colors
- CD-ROM drive
- Color monitor
- Interface for the mass spectrometer (Ethernet 10/100)

Hardware for operating system Windows Vista (x86)

- Adhere to the QUADERA® Release Notes.


Software

- Operating system Windows XP Professional with Service Pack 2 or 3
- Operating system Windows Vista Ultimate (x86)
- **Note:** No other Windows operating systems are supported. 64-bit Windows operating systems are not supported.

Getting Help

Calling Help

If you need help during your work, you may utilize the following resources:

1. Select the **Help** menu and click **Contents** or **Index**,
or
Press the function key [F1].
2. If the **Contents**, **Index** and **Search** tabs are not displayed in the Help window, click Show .
3. Perform one of the following steps in the Help window:
 - Click the **Contents** tab to display the table of contents for the help file.
 - Click the **Find** tab to search for specific key words. Enter the required words and then click Search.
 - Click the **Index** tab to search for specific words or to choose from a key word list.


You can control the number of the found topics by adding key words to the search string or by removing them from the string. This way you can restrict the search result in the list to the relevant topics and key words.

In addition, you can use the Windows start menu to open the online help:

1. Click on the Windows **START** button and select **Programs**.
2. Select the program group **QUADERA** and click on **QUADERA Help**.

Changing the Display of a Help Topic

The Help window uses the same settings for fonts, font colors and background colors as the browser installed on your computer. These settings and other options depend on the type and version of the installed browser. You can change the appearance of the help topics in the Help window by changing the settings for fonts and colors.

1. Open the Help window.
2. In the **Help** window, click **Options** and then **Internet Options** .
3. In the **General** tab, click **Accessibility** and then select **Ignore colors specified on Web pages**.
4. Click **OK**.
5. Perform one of the following actions in the **Internet Options** dialog box:
 - Changing the background or text color in the help:
In the **General** tab, click **Colors...** and then select the required options.
 - Changing the font in the help:
In the **General** tab, click **Fonts...** and then select the required options.


NOTE:

Any change in the font and background color of the help topics in the Help window will also affect the font and background color of websites displayed by Microsoft Internet Explorer.



Further information on the settings and options available in your browser can be found in the help file for your browser.

Printing a Help Topic

Printing the current topic

1. In the Help window, click **Print** .
2. Select the required printing options.

Printing several topics

1. In the Help window, click the **Contents** tab.
If the **Contents** tab is not displayed, click Show .
2. Select the required heading and then click Print .
3. Perform one of the following actions:
 - In order to print the current page, select **Print selected topic**.
 - In order to print all topics under the selected heading, select **Print the selected heading and all subtopics**.
4. Select the required printing options.

Further Information

You can check which version of QUADERA® is installed on your computer and determine the product ID and the license key of your program. In addition, you can call up system information.

- In the **Help** menu, select **About...**

Reporting Errors

QUADERA® allows you to create an error report which also contains additional comments from you. These reports are helpful to our support staff when solving problems.

- In the **Help** menu, click **Report an Error...** You are directly connected to an error report form on the website of QUADERA® (<http://www.quadera.net>). Please fill out this form carefully. Your error report will be automatically acknowledged if you quote a valid email address. You receive an email and a reference number for further queries on the status of your issue.

Installing and Uninstalling QUADERA

Installation Program SETUP

QUADERA® comes as a compressed file on a CD-ROM. SETUP copies and unpacks the QUADERA® program files and creates the required directories on the selected drive (pay attention to the system requirements).

The installation directory (default: C:\Program Files\QUADERA) contains all QUADERA® program files. Special subdirectories are created for all other files.

NOTE:

If required you can change the locations of the special subdirectories after the installation has been completed (menu Tools>Options).

SETUP is used for the following tasks:

- Installing QUADERA®,
- Updating QUADERA®,
- Upgrading QUADERA®.

NOTES:

Uninstalling QUADERA prior to installing a new version will most often result in the best installation.

Unrestricted use of QUADERA® requires a valid license key.

Installing

NOTE:

Unrestricted use of QUADERA® requires a valid license key.

NOTE:

In order to install QUADERA®, a user account with administrator access rights is required.

Proceed as follows to install QUADERA®:

1. Check to make sure that the system requirements are met.
2. Start Windows and close all other applications. Pay attention to the instruction manual for your operating system.
3. Insert the QUADERA® installation CD into the CD-ROM drive.
 - The installation procedure should start automatically after a few seconds.
 - If the installation procedure does not start within 30 seconds, the autostart function of the drive may be disabled. In this case, use Windows Explorer to access the CD-ROM drive and execute the **index.html** file.
4. Follow the instructions of the installation program and enter all required parameters or accept the respective default settings.

NOTE:

After installing QUADERA®, you have to set up the following:

- The communication between the PC and the mass spectrometer,
- The configuration of the mass spectrometer.

An account with administrator access rights is **not** required in order to operate QUADERA®.

Setting Up

NOTE: By default, QUADERA® works with a simulator that is installed together with the software. After the installation procedure, QUADERA® is basically ready for operation and it can be used without a device.

NOTE: Adhere to the QUADERA® Release Notes.

Proceed as follows to set up QUADERA®:

1. Start QUADERA®.
2. In the **Device** menu, click **Device Setup....** The "Device Setup" dialog opens. Click **Search**.
3. The search scans the network for running QMG mass spectrometers. Click **Search** again, if all mass spectrometers are not found, to start another search.
4. In the "Device Search" dialog select a device (or devices) and click **Add**. Close the dialog.
5. Click **Apply** in the 'Device Setup' dialog to acknowledge the input. QUADERA will now connect to each device, acquire the Device Name, and disconnect from each device.
 - Any device unable to connect will be named 'unknown'. On any future 'Connect', the Device Name will be acquired and assigned.
6. Click the **Configure** button to change the name of any device.
7. **Apply** any changes and close the dialog.
8. QUADERA® is now configured for the connection with the mass spectrometer(s).
9. If necessary adjust the configuration:
 - Use the basic device settings in the device status view ("Device Configuration View" icon) to adjust the configuration. Normally these settings have already been performed in the factory.

QUADERA® now allows more than one device to be connected and acquiring data simultaneously if properly licensed ('Multiplexing' license). This multiple device design, known as Multisensor, can run for an extended period of time but it is recommended to limit duration and/or quantity of data collected in any one session.

NOTE: Multisensor can be enabled through the Options menu and must be enabled to use the Multiplexing add-in.

Adjusting the Device Settings

NOTE:

Normally most device settings have already been performed in the factory. The Device Name is one setting that can be customized.

Proceed as follows to adjust the device settings:

1. Connect QUADERA® with the device.
2. In the device status view, click on the "Device Configuration View" icon. The "Device Configuration" window opens.
3. Adjust the parameters to the device settings. The following table list the available parameters.
4. Click [Close] to close the "Device Configuration" window.

NOTE:

Select only components that are actually installed in your device.

Parameter	Range	Description
• Device Name	Edit box	The Device Name used to label the device.
• Device MAC	Automatically detected	The unique hardware address of the device.
• Auto Connect at Startup	Dropdown list	Selection of feature to automatically connect device at QUADERA® startup.
• Analyser Detector Type	Dropdown list	Selection of the detector type (installed gauge head): <ul style="list-style-type: none"> • Faraday: only "Faraday" is available in recipes, • SEM: "Faraday" and "SEM" are available in recipes.
• Ion	Dropdown list	Selection of the ion source type:

Source Type	<ul style="list-style-type: none"> • Axial: Axial ion source (only QMG700), • Crossbeam: Cross-Beam ion source, • Grid: Grid ion source, • SPM: Sputter Process Monitor, • High sensitivity (only QMG220), • SpecPos (only QMG700), • SpecNeg (only QMG700). 	
• Protection	Dropdown list	<p>Monitoring of filament and SEM.</p> <p>If a pressure gauge is installed:</p> <ul style="list-style-type: none"> • InternalOff: use QUADERA® to switch filament and SEM manually on and off, • ExternalOnOff: an external system, such as a pressure gauge, protects filament and SEM. They are automatically switched on and off as determined by the parameters "Total Pressure Level On/Off". • ExternalOff: an external system, such as a pressure gauge, protects filament and SEM. They are automatically switched off as determined by the parameter "Total Pressure Level Off". Use QUADERA® to switch filament and SEM manually on.
• QMA	<p>For QMG220: Automatically detected</p> <p>For QMG700: Dropdown list</p>	<p>Indicates the installed QMA.</p> <p>Selection of the QMA.</p>
• QMH	<p>For QMG220: Automatically detected</p> <p>For QMG700: Dropdown list</p>	<p>Indicates the installed RF device, which defines the mass range.</p> <p>Selection of the QMH, depends on the installed QMA.</p>

<ul style="list-style-type: none"> • Mass Range 	<p>Automatically detected</p>	<p>Indicates the mass range in [amu], depends on the installed QMA and QMH.</p>
<ul style="list-style-type: none"> • Simulation Mode 	<p>Dropdown list</p>	<p>Defines the simulation mode of the device:</p> <ul style="list-style-type: none"> • Off, • Internal, • External. <p>NOTE: The software simulation (local simulation on the PC) requires no real device.</p>
<ul style="list-style-type: none"> • IO220, or IO700 	<p>Automatically detected</p>	<p>Indicates whether an Input/Output-module (IO220 or IO700) has been detected or not.</p>
<ul style="list-style-type: none"> • Total Pressure Level Off 	<p>Number > 0</p>	<p>Only valid when a total pressure gauge is installed.</p> <p>Monitoring the QMG via total pressure measurement: pressure threshold when filament and SEM switch automatically off (pressure rise).</p> <p>The parameters "Total Pressure Level Off" and "Total Pressure Level On" should form a hysteresis to avoid repeated switching when minor pressure fluctuations occur.</p>
<ul style="list-style-type: none"> • Total Pressure Level On 	<p>Number > 0</p>	<p>Only valid when a total pressure gauge is installed.</p> <p>Monitoring the QMG via total pressure measurement: pressure threshold when filament and SEM switch automatically on (decrease of pressure).</p>
<ul style="list-style-type: none"> • Total Pressure RS 485 Address 	<p>Valid address</p>	<p>Only valid when a total pressure gauge is installed.</p> <p>Total pressure measurement: address of the installed digital pressure gauge.</p> <p>Note that the pressure gauge is only recognized when the device is turned on (no "hot-plug").</p>
<ul style="list-style-type: none"> • Total Pressure 	<p>Automatically detected</p>	<p>Only valid when a total pressure gauge is installed.</p>

Type

Total pressure measurement: type of the installed analog/digital pressure gauge.

Note that the pressure gauge is only recognized when the device is turned on (no "hot-plug").

NOTE: Buttons are available to degas the Filament Ion Source and Total Pressure Gauge filament (if present). Degas of the Filament Ion Source can be started and stopped manually or run for a duration of time. The Degas function can also be accessed from the All Device Status View.

Version Number

The product version of QUADERA® is indicated by a two-digit number shown as x.yz, e.g. 1.12.

- "1" indicates the major version,
- "12" indicates the minor version.

In the **Help>About...** menu you find the version number of your software and further information, as well as product extensions.

Update

A software update is a maintenance release of the software within the same major version. The minor version has been increased (e.g. from 1.12 to 1.13). Updates contain new features and additional functions or they fix software bugs that have been discovered.

Upgrade

A software upgrade represents an extensive revision of the software and is marked as a new major version (e.g. from version 1 to 2). Upgrades contain extensive revisions and they offer an extended and improved range of functions for the software.

Updating

The version number allows you to find out if an update or upgrade for QUADERA® is available.

Proceed as follows to update/upgrade your QUADERA® version:

1. Start Windows and close all other applications.
2. Insert the CD with the latest product release into the CD-ROM drive.
3. Follow the instructions of the installation program and enter all required parameters or accept the respective default settings.

Uninstalling

NOTE:

In order to uninstall QUADERA®, a user account with administrator access rights is required.

Proceed as follows to uninstall QUADERA®:

1. Exit QUADERA®.
2. In the Windows Start menu, select **Control Panel > Add or Remove Programs**.
In Windows Vista: Start menu **Control Panel > Programs > Uninstall a program**
3. Select **QUADERA®**.
4. Click **[Remove]** or **Uninstall** (Vista). You are asked to confirm the action.
5. Click **[OK]** or **[Continue]** (Vista) to uninstall the QUADERA® application.

NOTE:

Files which have been created automatically by the software and user files remain on the harddisk. If you want to remove these files you may do so manually. In this case, adhere to the QUADERA® Release Notes.

Operating Concept

Basics for Operation

For a basic understanding of the operating routines and procedures in QUADERA® it is necessary to know the object structures that are visible to the user.

Object	Description
QUADERA®	Instance of the QUADERA® software
Toolboxes	The toolboxes provide tools which allow you to adjust the working area according to the measurement task.
Software device	Image of the real device in QUADERA®
Device	Mass spectrometer
Measurement project	<p>Contains all instruments required to perform a specific application.</p> <p>One device is assigned to each measurement task. It is possible that several measurement projects relate to the same device.</p>
Recipe	Sequence or collection of measurement tasks
Measurement task	Configurable measurement task. It is the basic component of a recipe and contains the measuring mode and all parameters required for its definition (e.g. MID, MCD, Scan).
Working area	<p>Part of the graphical user interface of QUADERA®. The working area is used for the following:</p> <ul style="list-style-type: none"> • To display the recipe editor. This working area is present in the most recipes and cannot be removed by the user. • As a container for the sections and the related measuring data displays. The user can add several working areas to a recipe.
Section	<p>Part of the working area</p> <p>Each working area - except for the working area used to display the recipe definition - can be divided into so-called sections by the user. Each section can be filled with a graphical object (e.g. measuring data display).</p>

Chart element	Graphical object which connects the data of a measurement task with a data display. A chart appears in the section.
---------------	---

The data display in QUADERA® is strongly related to the corresponding measurement tasks. The appropriate tool allows you, for instance, to create or remove a measurement task directly in the data display of the section.


Example for the relation between measurement task and data display

In order to observe the change of several gases with time, the MID (Multiple Ion Detection) type of measurement is especially suitable. In this example, one measurement task relates to a mass whose intensity is to be measured, and it defines the parameters required for the measurement. The recipe unites all measurement tasks, i.e. the masses to be observed. During a measurement, the measurement tasks are performed one after the other, the readings are collected and stored in the related measurement project. The repeated execution of a measurement task results in a sequence of data which show the course of the related mass signals as a function of the time. The measuring data which are obtained in a measurement task can be displayed graphically in a chart in the section (e.g. as a curve or a bar chart). As a result, they represent a chart element.

Operating Elements





User Interface

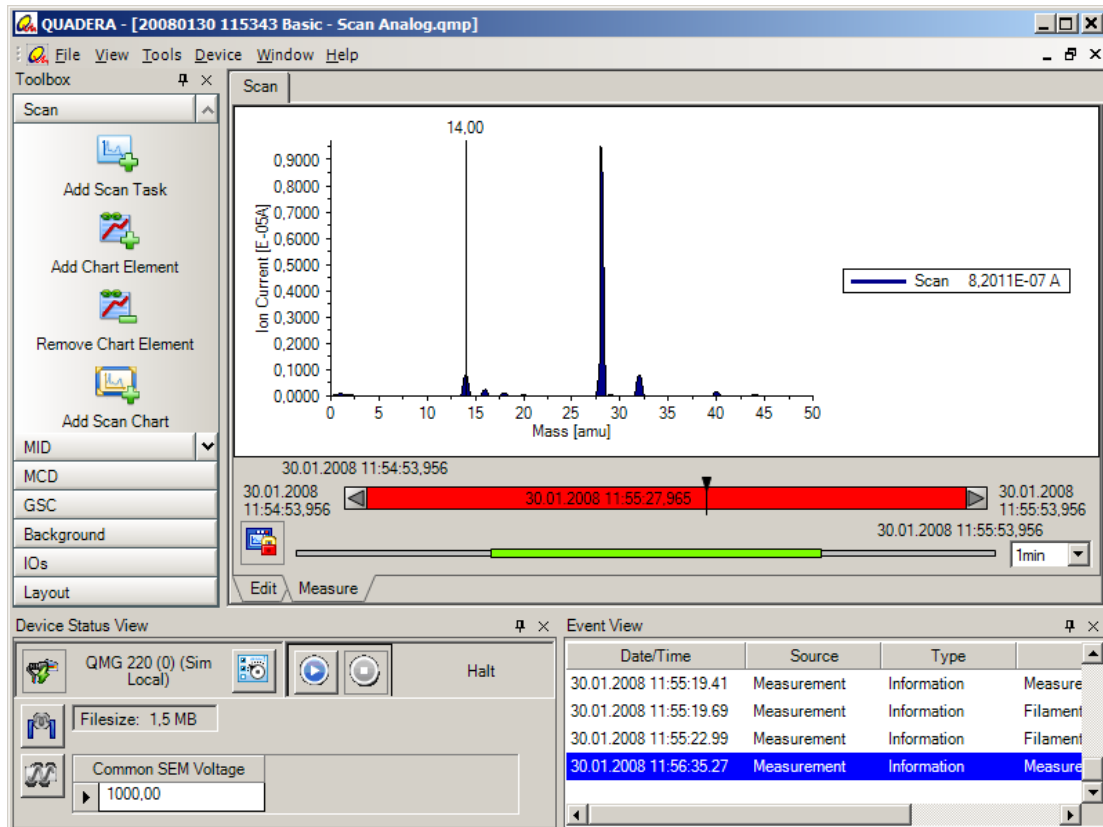The QUADERA® window is divided into several areas. For each area, a tooltip displays brief information. For this, move the mouse pointer to the required area in the figure below. For more detailed information, click the respective area.



Example of the QUADERA® user interface

Screen Elements

Name	Example	Description
Checkbox		<p>You can select Yes (with checkmark) or No (without checkmark) as follows:</p> <ul style="list-style-type: none"> • Press the space bar, • Click the checkbox with the mouse.
Radio buttons		<p>Radio buttons allow you to select one option at a time. You can select the required option as follows:</p> <ul style="list-style-type: none"> • Press the space bar, • Click the required button with the mouse. <p>This will automatically reset the previously selected button.</p>
Dropdown list		<p>Select the required list item as follows:</p> <ul style="list-style-type: none"> • Click the currently displayed item to open the entire dropdown list, • Click the required item with the mouse. The dropdown list closes and only the selected item is displayed.
Spin buttons		<p>Increase or decrease the displayed value as follows:</p> <ul style="list-style-type: none"> • Click one of the spin buttons to increase (arrow up) or decrease (arrow down) the value by one, • Click the input field next to the spin buttons and enter the required value directly.

Tooltips

Device configuration view.

The tooltip is a small box in the graphical user interface and displays supplementary information on an item, such as symbols. A tooltip appears when the user hovers the mouse pointer over an item, without clicking it.

Mouse Actions

Action	Description (default assignment for the mouse buttons)
Click	Position the mouse pointer on the required object (file, text, figure etc.). Then press the left mouse button.
Double-click	Position the mouse pointer on the required object. Then press the left mouse button twice in rapid succession.
Drag & drop	Position the mouse pointer on the required object. Press the left mouse button and keep it pressed. Drag the object to the new position (destination) and then release the mouse button. The object will be put down at the destination.
Right mouse button	Position the mouse pointer on the required object. Then press the right mouse button. In general, this will open a context menu offering some object related functions to you.

Keyboard Shortcuts

NOTE:

The following table describes the default settings for the keyboard shortcuts. You can customize the keyboard shortcuts to suit your needs.

Key	Action
F1	Call up help
CTRL+O	Open a measurement project
ALT+F4	Exit the application
ALT+F8	Call up the Macros... dialog

Customizing the Keyboard Shortcuts

By default, QUADERA® already contains predefined keyboard shortcuts. You may change or extend these settings to suit your needs. As an example, you may do one of the following:

- Assign keyboard shortcuts to frequently used commands and macros,
- Delete keyboards shortcuts which are no longer needed.

Assigning keyboard shortcuts

Proceed as follows to assign a keyboard shortcut:

1. Call up the context menu for the menu bar.
2. Click **Customize...**
3. Click **Keyboard...**
4. Select a command category from the list.
5. Click a command in the command list. The **Specify a Shortcut** field displays the keyboard shortcut that is currently assigned to the selected command.
6. Select a keyboard shortcut in the **Specify a Shortcut** field.
7. Click **Assign**. The keyboard shortcut is assigned to the selected command.

If the selected keyboard shortcut has already been assigned to another command, the latest assignment will replace the previous one.

Click **Reset All...** to reset all keyboard shortcuts to the default assignments.

Deleting keyboard shortcuts

Proceed as follows to delete a keyboard assignment:

1. Call up the Context menu for the menu bar.
2. Click **Customize...**
3. Click **Keyboard...**
4. Select a command category from the list.

5. Click a command in the command list. The **Specify a Shortcut** field displays the keyboard shortcut that is currently assigned to the selected command.
6. Click **Remove**. The assignment between the keyboard shortcut and the command is removed.

Click **Reset All...** to reset all keyboard shortcuts to the default assignments.

User Interface

Title Bar

The title bar is a subarea of the QUADERA® user interface.

The title bar displays the following items:

- Program symbol: Click this symbol to call up the title bar menu.
- Program name
- Currently loaded file (measurement project)

Menu Bar

The menu bar is a subarea of the QUADERA® user interface.

Each menu contains a list of commands. The menu bar allows you to call up all functions of QUADERA®. The following main menus are available:

File	File and printer related functions
View	View settings
Tools	Additional functions
Device	Device related functions
Window	Management and arrangement of the windows
Help	Help functions

QUADERA® main menus

File menu

The **File** menu contains the following functions:

- Open
- Export
 - ASCII
- Save as Template...
- Close
- Recent Files
- Exit

View menu

The **View** menu contains the following functions:

- Show Start Page
- Event View
- Device Status
- All Device Status
- Toolbox

Tools menu

QUADERA HTML Help

The **Tools** menu contains the following functions:

- Programming
 - Macros...
 - Create Add-in...
 - Add-in Manager...
- Options...
- Spectra Library

Device menu

The **Device** menu contains the following functions:

- Connect
- Run
- Device Setup...

Window menu

The **Window** menu contains the following functions:

- Arrange Icons
- Cascade
- Close All Windows
- Tile Horizontally
- Tile Vertically
- Minimize All Windows
- Window List

Help menu

The **Help** menu contains the following functions:

- Contents
- Index
- Report an Error...
- About...

Options

Use the "Options..." window to perform the following settings:

- Specifying the path (file location) for various file types used by Quadera® ("File Locations" tab)
- Changing the line thickness of curves in charts ("Display" tab)
- Enabling Multisensor, the ability to connect to and collect from more than one device. As of QUADERA version 4.20 this must be enabled (and licensed) to use either Multisensor or Multiplexing (from VSTA).

Toolbox

Toolbox

The toolbox is a subarea of the QUADERA® user interface.

The toolbox is used to customize the working area of a measurement project. The main task is to create new objects. The toolbox is subdivided into different groups according to the subject. One tool can be used in several groups. Click the respective button to open the required toolbox.





NOTE:

Toolboxes may contain varying tools depending on the configuration of QUADERA®.

Refer to the alphabetical list of tools if you search for a specific tool.

Applying Tools









Applying via drag & drop






1. Open the required toolbox.
2. Use the buttons  and  if necessary. The toolbox is scrolled up and down, respectively, to display the desired tool.
3. Drag the required tool into the section:
 - A mouse pointer shaped as  indicates that the selected tool is applicable,
 - A mouse pointer shaped as  indicates that the selected tool is not applicable.











Alphabetical list of tools

List of Tools

Alphabetical list of all tools which are available in QUADERA®:

Icon	Name	Description
	Add 'Analog Input' Editor	Add an analog input editor to the section.
	Add Analog Input Task	<p>Depends on the working area into which you drag the tool:</p> <ul style="list-style-type: none"> • Dragging the tool to the recipe editor: Add a measurement task to the recipe. The task uses an analog input channel, such as the quadrupole controller QC ("EXT IN"). • Dragging the tool to the chart: Add a measurement task to the recipe using an analog input channel. Display the data of this measurement task in the chart. <p>Refer to the operating instructions of your QMG mass spectrometer.</p>
	Add 'Analog Output' Editor	Add an analog output editor to the section.
	Add Chart Element	Connect an existing measurement task with a chart.
	Add 'Digital Input' Editor	Add a digital input editor to the section.
	Add 'Digital Output' Editor	Add a digital output editor to the section.
	Add MCD Chart	<p>Add an (empty) MCD chart to the section.</p> <p>Only available for MID recipes.</p>
	Add MCD Task	<p>Depends on the working area into which you drag the tool:</p> <ul style="list-style-type: none"> • Dragging the tool to the recipe editor: Add a MCD measurement task to the recipe. • Dragging the tool to the chart:

		<p>Add a MCD measurement task to the recipe. Display the data of this measurement task in the chart.</p> <p>Only available for MCD recipes.</p>
	Add MID Chart	<p>Add an (empty) MID chart to the section.</p> <p>Only available for MID recipes.</p>
	Add MID Task	<p>Depends on the working area into which you drag the tool:</p> <ul style="list-style-type: none"> • Dragging the tool to the recipe editor: Add a MID measurement task to the recipe. • Dragging the tool to the chart: Add a MID measurement task to the recipe. Display the data of this measurement task in the chart. <p>Only available for MID recipes.</p>
	Add Peak Task	<p>Depends on the working area into which you drag the tool:</p> <ul style="list-style-type: none"> • Dragging the tool to the recipe editor: Add a peak measurement task to the recipe. • Dragging the tool to the chart: Add a peak measurement task to the recipe. Display the data of this measurement task in the chart. <p>Only available for scan recipes (see recipe parameter "Mass Mode").</p>
	Add Scan Chart	<p>Add an (empty) scan chart to the section.</p> <p>Only available for scan recipes.</p>
	Add Scan Task	<p>Depends on the working area into which you drag the tool:</p> <ul style="list-style-type: none"> • Dragging the tool to the recipe editor: Add a scan measurement task to the recipe. • Dragging the tool to the chart: Add a scan measurement task to the recipe. Display the data of this measurement task in the chart.

		Only available for scan recipes (see recipe parameter "Mass Mode").
	Add Total Pressure Task	<p>Icon only available for QMG220.</p> <p>Depends on the working area into which you drag the tool:</p> <ul style="list-style-type: none"> • Dragging the tool to the recipe editor: Add a new total pressure measurement task to the recipe. • Dragging the tool to the chart: Add a total pressure measurement task to the recipe. Display the data of this measurement task in the chart.
	Add Working Area	Create a new working area in the current recipe or measurement project.
	Remove Chart Element	Delete a measuring line or a measurement task from the chart.
	Remove Section	Delete the selected section.
	Remove Section Content	Delete all objects of a section, such as charts and measurement tasks etc.
	Remove Working Area	Delete the current working area.
	Split Section Bottom	Split the section in half horizontally. A new section is added to the bottom of the present contents.
	Split Section Left	Split the section in half vertically. A new section is added to the left of the present contents.
	Split Section Right	Split the section in half vertically. A new section is added to the right of the present contents.
	Split Section Top	Split the section in half horizontally. A new section is added to the top of the present contents.

Measurement Project Window

The measurement project window is a subarea of the QUADERA® user interface.

The measurement window is used to display a measurement project and contains the following areas:

- Recipe selection,
- Working area,
- Working area selection.

Recipe Selection

The recipe selection is a subarea of the measurement project window.

The recipe selection tab allows you to switch to a recipe within a measurement project.

Working Area

The working area is a subarea of the measurement project window or of a recipe.

The working area is used for displaying measuring data and for editing the currently selected recipe. The recipe editor is present in every recipe and cannot be removed by the user. Additional display areas serve as containers for the related measuring data displays. The user can add several display areas to a recipe.

Working Area Selection










The working area selection is a subarea of the measurement project window.

Several working areas are available for each recipe. The working area selection tabs allow you to switch between the displays.

Device Status View

The device status view is a subarea of the QUADERA® user interface.

The device status view shows the most important device parameters and states. At a glance, you can see all the important information on the status of the connected device, the measurement and the recipe. The displayed icons and parameters are predetermined and cannot be hidden. Use the icons to easily access the basic functions of the software and the device:

Icon	Description
	Device disconnected. Click on the icon to connect the device.
	Device connected. Click on the icon to disconnect the device.
	Basic device settings. Click on the icon to view the basic device settings in the "Device Configuration" window, and edit as appropriate.
	Measurement stopped. Click on the icon to start the measurement.
	Measurement running. Click on the icon to stop the measurement.
	Filament off. Click on the icon to switch the filament on.
	Filament on. Click on the icon to switch the filament off.
	SEM off. Click on the icon to switch the SEM on.
	SEM on. Click on the icon to switch the SEM off.

Common SEM Voltage

Common operating voltage of the SEM. Enter the required value or use the spin buttons. Measurement tasks will use the "Common SEM Voltage" if <<SEM-Voltage>> is selected from the dropdown list for the corresponding recipe parameter "SEM Voltage".

NOTE:

The "Common SEM Voltage" parameter is not available when the Faraday-Cup has been selected in the basic device settings (Symbol "Device Configuration View").

All Device Status View

The All Device Status View is a subarea of the QUADERA® user interface.

The All Device Status View shows a collection of the most important device parameters and states for all devices connected to QUADERA. At a glance, you can see all the important information on the status of the connected device, the measurement and the recipe. The displayed icons and parameters are predetermined and cannot be hidden. Use the icons, described on the Device Status View page, to easily access the basic functions of the software and the device.

The All Device Status View allows for selection of multiple devices (using CTRL or Shift key) and provides a context menu for selection of functions. The All Device Status View is most useful for viewing status when operating QUADERA in the Multiplexing mode.

Please note that the All Device Status View does not replace the Start Page as the main control. You must still use the Start Page and its Device icons to access Projects and Templates for a Device.

Event View

The event view is a subarea of the QUADERA® user interface.

The event view informs you of events that have occurred for each device (the selected device on the Start page). Warnings, informations and errors are displayed in a compact way.

Events related to measurement, device and system are listed. The presentation follows the event view used by the Windows operating system. Refer to the list of events for a detailed description.

Context Menus

Context Menus

A context menu is a special menu that opens up when pressing the right mouse button. It is context sensitive and always contains commands which are related to the currently used screen area.

In QUADERA®, you may call up context menus in the following screen areas:

Title bar	Context menu with functions relating to the QUADERA® window.
Window title	Context menu with functions relating to the respective window in QUADERA®.
Menu bar	Context menu with functions relating to the menu bar settings.
Recipe Selection	Context menu used for adjusting the recipe layout (working area)
Frame of the section	Context menu used for showing and hiding the navigator.
Charts in the working area	Context menus with functions used for adjusting the chart layout.





Context menus in QUADERA®

Calling Up a Context Menu

1. Position the mouse pointer in the required screen area.
2. Press the right mouse button.

Context Menu "Title Bar"

Click with the right mouse button into the title bar of a window. The context menu "title bar" appears. It contains the following functions:

	Restore	Restore the default size for the selected window.
	Move	Move the window.
	Size	Change the window size.
	Minimize	Minimize the window size.
	Maximize	Maximize the window size.
	Close	Close the window or the application.

Context Menu "Menu Bar"

Click with the right mouse button into the menu bar. The context menu "Menu bar" appears. It contains the following functions:

- Lock the Toolbars Checkbox: Determine whether or not it is possible to change the positions of the menu bars.
- Customize... Open a window which allows you to customize or create menu bars, and also to configure keyboard shortcuts.

Context Menu "Recipe Selection"

Click with the right mouse button into the recipe selection area. The context menu "Recipe Selection" appears. It contains the following functions:

- **Rename selected tab** Open the dialog field "Rename selected tab" to rename the tab of the selected working area.

Context Menu "Frame of the Section"

Click with the right mouse button into the frame of the section. The context menu "Frame of the section" appears. It contains the following functions:

- Show Navigator Show or hide the data navigator.
- Rename selected tab Open the dialog field "Rename selected tab" to rename the tab of the selected working area.

Context Menu "Chart"

Click with the right mouse button into a chart located in the working area. Various context menus are available, depending on the selected mouse pointer position:

- Click on the measuring data display. Context menu "Chart" appears. It contains the following functions:
 - Zoom Out
 - Reset Zoom
 - Hold
 - Legend
 - Print
 - Enable Background Subtraction
 - Enable Reference Subtraction
 - View as Partial Pressure
 - Marker (only in MID/MCD recipes)
 - Display (only in MID/MCD recipes)
 - Analog I/O Characteristics
- Click on the x-axis. Context menu "Axis X" appears.
- Click on the y-axis. Context menu "Axis Y" appears.
- Only when the legend is shown: Click on the chart legend. Context menu "Legend" appears.
- Only for trending charts in MID/MCD recipes: Click on the right y-axis. Context menu "Axis Y2" appears.

Context menu "Chart"

Click on the measuring data display to open this context menu.

- Zoom Out Undo the last zoom action.
- Reset Zoom Undo all zoom actions, i.e. reset the display to the initial area.
- Hold
 - Enabled (with checkmark):
Freeze the display during a measurement (no scaling and scrolling). Measuring data are still recorded and stored. "Hold On" is automatically selected when zooming or moving the cursor.
 - Disabled (no checkmark):
Disable the hold function and resume to display the recording of data. "Hold Off" is usually applied after zooming or moving the cursor.

NOTE: There is one hold function for each working area.

- Legend
 - Enabled (with checkmark):
The chart legend is displayed.
 - Disabled (no checkmark):
The chart legend is not displayed.
- Print
 - Print this Item: Prints the chart displayed.
 - Print Full Report: Prints a report based on the Print Preferences.
 - Set Print Preferences: Allows selection of items to print in the Full Report.
 - Print Preview: Provides a preview of what will be printed in the Full Report.
- Enable Background Subtraction

Allows Background Subtraction to be enabled and disabled.
- Enable Reference Subtraction

Allows Reference Subtraction to be enabled and disabled in a Reference Subtraction measurement project.
- View as Partial Pressure

Allows viewing MID data as Partial Pressure (or Amps).
- Marker

Only available for trending charts in MID/MCD recipes:

 - Enabled (with checkmark):
Displays the individual measuring points and the connecting lines.
 - Disabled (no checkmark):
Displays the connecting lines of the measuring points.
- Display

Only available for MID/MCD recipes.
Switch the representation of the chart:

 - Trend:
Continuously display the measuring data as a function of the time (in the selected section, see data navigator).
 - Bar:
Display the measuring data in a bar graph at the time specified by the cursor, see data navigator.
 - Table:
Display the measuring data in a table at

the time specified by the cursor, see data navigator.

- Analog I/O Characteristics Allows assignment of a characteristic to an Analog I/O (if available).

Context menu "Axis X"

Click on the x-axis to open this context menu. It is used to switch the presentation of the x-axis.

- Fixed Range of the axis is fixed
Only in scan recipes
- Automatic Range of the axis is adjusted to the measured values
Only in scan recipes
- Time Absolute Display the absolute time (date, time)
Only in MID/MCD recipes
- Time Relative Display the relative time (measuring time)
Only in MID/MCD recipes

Context menu "Axis Y"

Click on the y-axis to open this context menu. It is used to switch the presentation of the y-axis.

- Linear Linear axis scaling
- Logarithmic Logarithmic axis scaling
- Fixed Range of the axis is fixed
- Automatic Range of the axis is adjusted to the measured values

Context menu "Axis Y2"

This context menu is available only in MID/MCD recipes, and at least one measurement task is assigned to the second y-axis (via context menu "Legend"). Click on the right y-axis to open this context menu. It is used to switch the presentation of this axis.

- Linear Linear axis scaling
- Logarithmic Logarithmic axis scaling
- Fixed Range of the axis is fixed
- Automatic Range of the axis is adjusted to the measured values

Context menu "Legend"

This context menu is available only when the chart legend is shown

(via context menu "Chart"). Click on a measurement task in the legend to open this context menu.

- Chart Element Indicates the measurement task related to the invoked context menu.
- Axis Y1 The measuring data display of the indicated measurement task uses the left y-axis. You can define the y-axis for each measurement task, i.e. if the left or right y-axis is used for this task.

Only for MID/MCD recipes
- Axis Y2 The measuring data display of the indicated measurement task uses the right y-axis. Context menu "Axis Y2" becomes available. You can define the y-axis for each measurement task, i.e. if the left or right y-axis is used for this task.

Only for MID/MCD recipes
- Color... Opens the "Color" dialog to select the color for the chart display of the measurement task (curve color).

Note that you can also define the line thickness of the curve.

Context Menu "Docking Window"

NOTE:

This context menu is only available for the docking windows (Toolbox, Device Status View, All Device Status View, Event View), but not for the measurement project window and the start page.

Click with the right mouse button into the docking window title. The context menu "Docking Window" appears. It contains the following functions:

- Dockable Checkbox: Specify if the selected docking window is dockable or not.
 - No:
The behavior of the docking window is the same as known from a normal window. It appears in the window list, in the bottom part of the Window menu.
 - Yes:
When you move the docking window various anchoring points are displayed on the user interface. The "Floating" property is automatically assigned to the docking window if you do not move it on an anchoring point. Note that you can move the toolbox only to the displayed anchoring points.
- Hide Checkbox: Specify if the selected docking window is shown or hidden. Use the View menu to show a hidden window.
- Floating Checkbox: Specify if the selected docking window can be moved freely (even outside of the window of the related application).

Note:
 - "Floating" docking windows are always "Dockable",
 - The "Floating" property can not be assigned to the toolbox.
- Auto Hide Checkbox: Specify if the auto-hide function is enabled for the selected docking window, i.e. the corresponding docking window will be automatically hidden and shown if needed.

Capturing Screenshots of the User Interface

As a written documentation for your measurement projects you can capture and print out screens of the QUADERA® user interface. Proceed as follows:

1. Capture the screen. The screenshot is copied into the Windows clipboard:
 - Full screen capture: press the key combination "CTRL+Print",
 - Active window capture: press the key combination "CTRL+ALT+Print".
2. Open a suited image editor, e.g. Microsoft Paint (Windows start menu > Programs > Accessories > Paint).
3. Paste the screenshot from the Windows clipboard into the image editor, e.g. press the key combination "CTRL+V".
4. Use the image editor to print out the screenshot.

NOTE:

Various screen capture tools are available as freeware, shareware, and by purchasing. In general, these tools provide enhanced screen capture features compared to the procedure described above.

Getting Started

Starting QUADERA®

You can start QUADERA® from the Windows Start menu or from the desktop.

Windows Start menu

1. Click the Windows **Start** button and select the **All Programs** entry.
2. Select the **QUADERA** program group and click the **QUADERA** entry.

Desktop

You can start QUADERA® from the desktop if a shortcut has been created for the desktop during installation.


1. Double-click the **QUADERA** shortcut symbol on your desktop.

After starting QUADERA®, the start page is displayed.

Start Page

The Start Page selection (File or a Device) determines what is displayed within the views of QUADERA® (e.g. Measurement Projects, Event View, Device Status View, title bars, etc.). For example, select a device on the start page to see its Event View.

After starting QUADERA®, the start page is displayed. Here you can perform one of the following actions:

- Open existing measurement projects (*.qmp files) and work with them:
 -  Click on the **File** icon. All measurement projects that have been worked on recently are shown in a list. Select the required project and open it with **OK** or by double-clicking it.
 - Click the **More...** button to open a measurement project that is not present in the list.
- Selecting templates to start new measurements:
 - Click on the icon for the required device (Simulator or real device).
 - If you want to start a new measurement: Click on the "Templates" bar and select the desired template (measurement project templates *.qmt in the "Templates" list).
 - If you want to calibrate the device: Click on the "Calibration and Tuning" bar and select the desired template (calibration templates *.qmt in the "Calibration and Tuning" list).
 - Only QMG220: If you want to start a new RGA application (Residual Gas Analysis): Click on the "RGA Application" bar and select the desired template (measurement project templates *.qmt in the "RGA Application" list).

If the start page is not displayed, you can call it up as follows:

- In the **View** menu, click **Show Start Page**. The start page is displayed.
- Only if the start page is already open: In the **Window** menu, click the respective item in the list of open windows.

NOTE:

Continuing the measurement using an existing measurement project is not possible.

Example of a Measurement

Introduction

The goal of this sample measurement is to analyze the composition of air. For this, we do not perform a real measurement in vacuum. Instead, we are going to use the simulation mode of QUADERA® and the stored simulation data which represent a typical measurement of air with a Faraday detector. Except for small details, the course of a measurement is the same for all mass spectrometers.

Course of a Measurement - Scan

NOTE:

For software training and in order to practice the measurement runs we recommend that QUADERA® be used in the simulation mode.

The scan measurement type (ion current as a function of m/e) is suitable for obtaining an overview of all present gases.

1. Open the start page: In the **View** menu, click **Show Start Page**.
2. Click on the icon for the required device.
3. Create a new measurement project: In the "Templates" list, double-click e.g. **Airdemo Scan Analog.qmt**. This way you create a new measurement project based on the selected template.
Please note: The file extension for templates is *.qmt
4. The new measurement project window appears. The working area displays the scan project.
 - Edit the recipe (if necessary): Click the **Edit** tab.
 - Display the measuring data: Click the **Measure** tab.

NOTE:

You can start the measurement regardless whether the recipe editor or the working area has been selected.

5. Start the measurement: In the device status view, click on the "Start" icon. The connection to the device is automatically established. The device now receives the parameters for the current measurement task. You can adjust the chart layout while the measurement is running.
6. Stop the measurement: In the device status view, click on the "Stop" icon.
7. Close and save the measurement project. In the **File** menu, click **Close**. You are requested if you want to save the measurement project. QUADERA® suggests an automatically generated file name that is based on date/time of the measurement and the used template.
 - Yes: the "Save As" window used for saving measuring data opens up. Select a suitable name and path and then click **Save**. The measurement project will be saved and closed.
Please note: The file extension for measurement projects is *.qmp
 - No: the measurement project will be closed without saving the data.
 - Cancel: the action is cancelled. You will return to the measurement project without saving the data.

Course of a Measurement - MID

NOTE:

For software training and in order to practice the measurement runs we recommend that QUADERA® be used in the simulation mode.

The MID measurement type (Multiple Ion Detection) is suitable for observing changes of several gases with time.

1. Open the start page: In the **View** menu, click **Show Start Page**.
2. Click on the icon for the required device.
3. Create a new measurement project: In the "Templates" list, double-click e.g. **Airdemo MID.qmt**. This way you create a new measurement project based on the selected template.
Please note: The file extension for templates is *.qmt
4. The new measurement project window appears. The working area displays the MID project.
 - Edit the recipe (if necessary): Click the **Edit** tab.
 - Display the measuring data: Click the **Measure** tab.

NOTE:

You can start the measurement regardless whether the recipe editor or the working area has been selected.

5. Start the measurement: In the device status view, click on the "Start" icon. The connection to the device is automatically established. The device now receives the parameters for the current measurement task. You can adjust the chart layout while the measurement is running.
6. Stop the measurement: In the device status view, click on the "Stop" icon.
7. Close and save the measurement project. In the **File** menu, click **Close**. You are requested if you want to save the measurement project. QUADERA® suggests an automatically generated file name that is based on date/time of the measurement and the used template.
 - Yes: the "Save As" window used for saving measuring data opens up. Select a suitable name and path and then click **Save**. The measurement project will be closed and saved.
Please note: The file extension for measurement projects is *.qmp
 - No: the measurement project will be closed without saving the data.
 - Cancel: the action is cancelled. You will return to the measurement project without saving the data.

Chart Display

In the working area selection, click the **Measure** tab (or the tab which corresponds to the required working area). The measuring data of the project are displayed in the section (chart display):

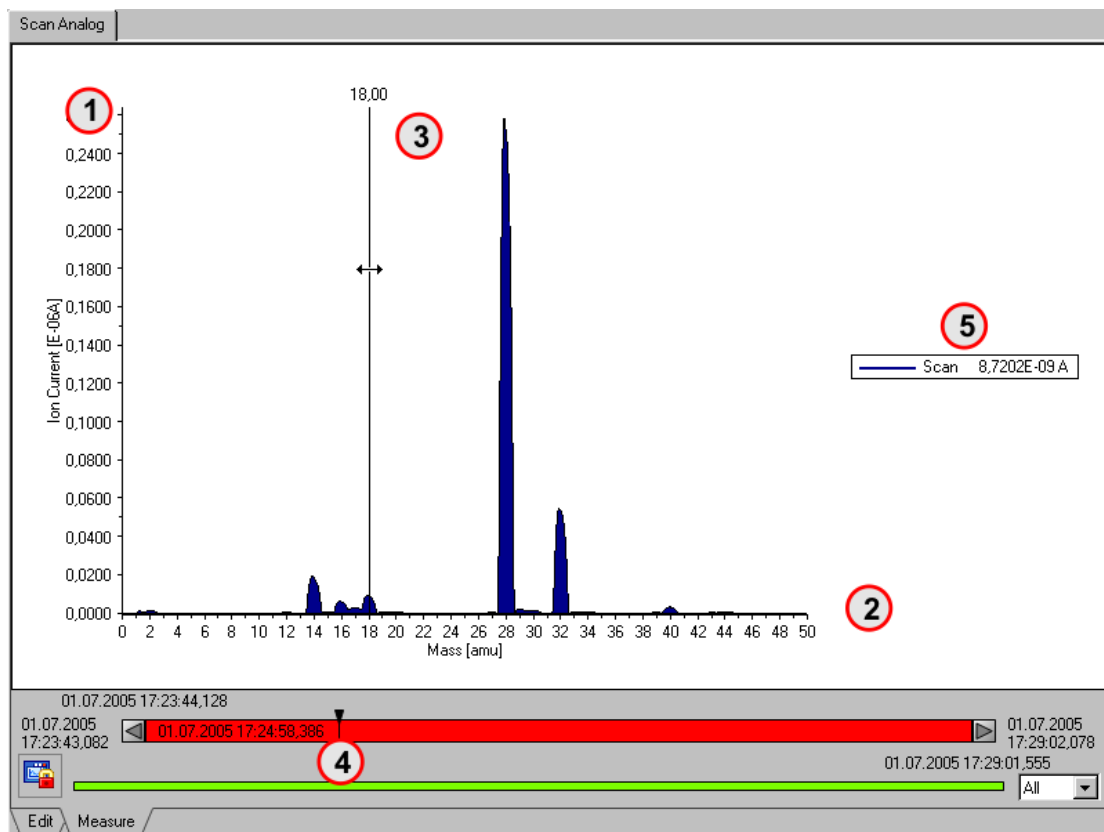


Chart display (example)

- 1 - Y-axis
- 2 - X-axis
- 3 - Cursor, indicates the x-axis position (mass)
- 4 - Data navigator
- 5 - Legend (measuring value at the cursor position)


- You can navigate in the measuring data by means of the data navigator or by pulling the cursor (mouse pointer is displayed as a double arrow).
- The context menus for the chart gives you access to additional functions.
- Use the tools "Add Chart Element" and "Remove Chart Element" to add and delete existing measurement tasks to and from the chart, respectively.

Data Navigator

Data Navigator

You can show and hide the data navigator by means of the context menu "frame of the section".

The data navigator is located below the measurement display. It allows you to scroll through the measuring data along the time axis. This is possible while a measurement is running and also for stored measuring data. If a measurement is running, this will automatically freeze the display (hold mode). You can exit the hold mode with the **Hold Off** function, e.g. by clicking on the "Hold Mode" icon.



Data navigator

The data navigator contains the following parts:

- The lower navigator bar comprises the entire measurement period. Use the dropdown list to the right of the bar to select the required period. This period will be represented by a green scroll bar.
 - Time period ("1 min"... "4 weeks"): The measuring values of the selected time period can be displayed.
 - All: All measuring values can be displayed.
- The upper navigator bar comprises the time period that has been selected in the lower navigator bar (green bar). The range limits are displayed at the left and right end of the bar.
- The red scroll bar inside of the upper navigator bar comprises a time period whose range limits are displayed at the upper left and lower right end of the bar (it covers 1 minute in the above example "Data navigator").
- The cursor in the upper navigator bar (vertical line) is used to determine which point of time is to be displayed in the chart. This point of time is displayed next to the cursor.

Icon "Hold Mode"



"Hold On": the display is frozen (hold mode is on).

Click on the icon to exit the hold mode.



"Hold Off": the display is updated (hold mode is off).

Click on the icon to activate the hold mode.

Using the data navigator

The data navigator allows you to quickly access the entire measurement period. You can easily move the time window displayed in the chart across the entire navigation area. The measurement displays in different sections are synchronized.

Most measurements cover a rather restricted period of time. For this reason, the lower navigator bar is only rarely used. The two-bar design is only required for improved navigation when handling very large amounts of data.

- Data navigator and zooming
- Data navigator in scan measurements
- Data navigator in MID/MCD measurements

Data Navigator and Zooming

Scan measurements

In a scan measurement, the data navigator refers to the chronological order of the individual scans (measuring cycles). This is useful when navigating between the individual measuring cycles. The zoom function applies to the scan displayed in the chart (intensity as a function of the mass) and is independent of the data navigator.

The selected magnification is maintained if you select another measurement cycle or change the time period with the data navigator.

MID/MCD measurements "Trend"

In the "Trend" view, the data navigator displays the time period of the zoomed detail. The red scroll bar in the upper data navigator is synchronized with the zoom function of the x-axis (time).

The selected magnification is maintained if you move the time period displayed in the chart with the data navigator, or if you change the time period.

MID/MCD measurements "Bar"

In the "Bar" view, the cursor position in the data navigator specifies the point in time for which the measuring data are displayed. In a bar graph, the zoom function is independent of the data navigator and it applies to the intensity (y-axis) only.

The selected magnification is maintained if you move the time period displayed in the chart with the data navigator, or if you change the time period.

MID/MCD measurements "Table"

There is no zoom function available in the "Table" view. The data in the table represent the measured values at the time that is indicated by the cursor position in the data navigator.

Data Navigator in Scan Measurements

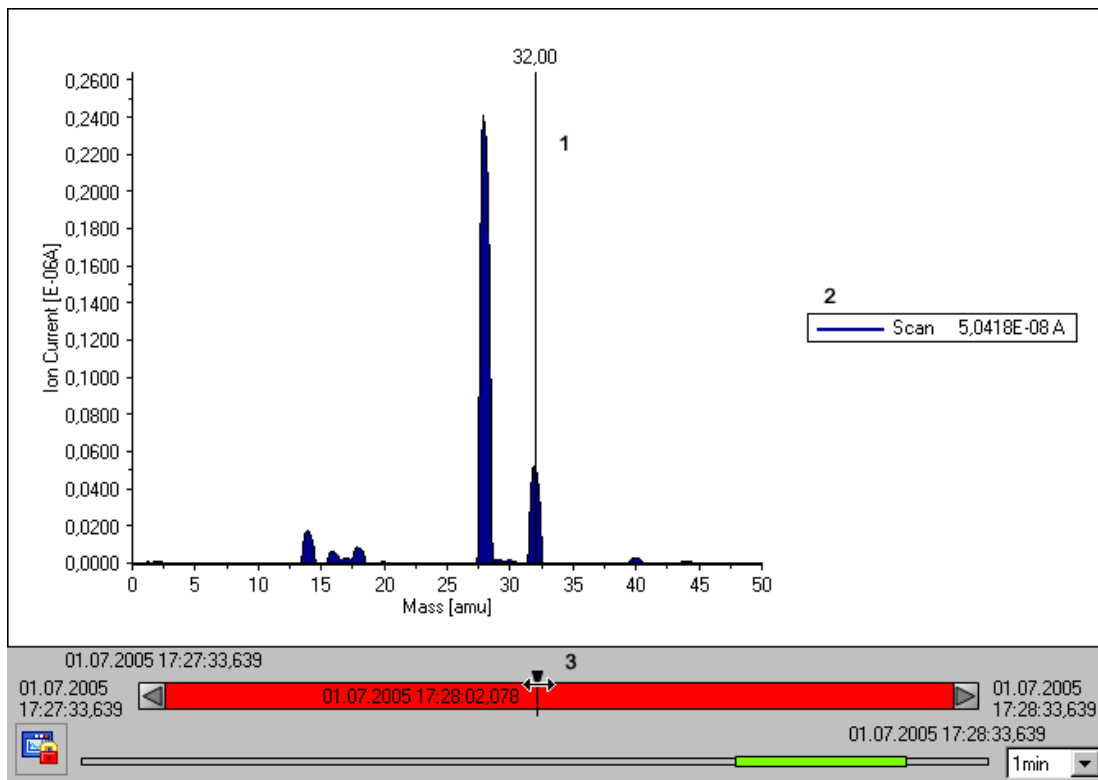


Chart display: Example of a scan measurement

The chart displays a scan (intensity as a function of the mass) at a point in time which is specified by the cursor position in the data navigator (item 3 in the above figure). It is only possible to display the scans in the time period specified by the red scroll bar in the upper navigator bar.

The measuring values displayed in the chart are determined by the cursor positions in the data navigator and in the chart. The following rules apply:

- The cursor in the upper navigator bar (item 3) determines which scan is to be displayed in the chart, i.e. the point in time of a scan within the entire measurement period (measurement cycle).
- The cursor in the chart (item 1) determines the mass (x-axis) in the displayed scan for which the measuring values are listed (item 2).

Data Navigator in MID/MCD Measurements

Select the required chart view using the "Diagram" context menu.

"Trend" view

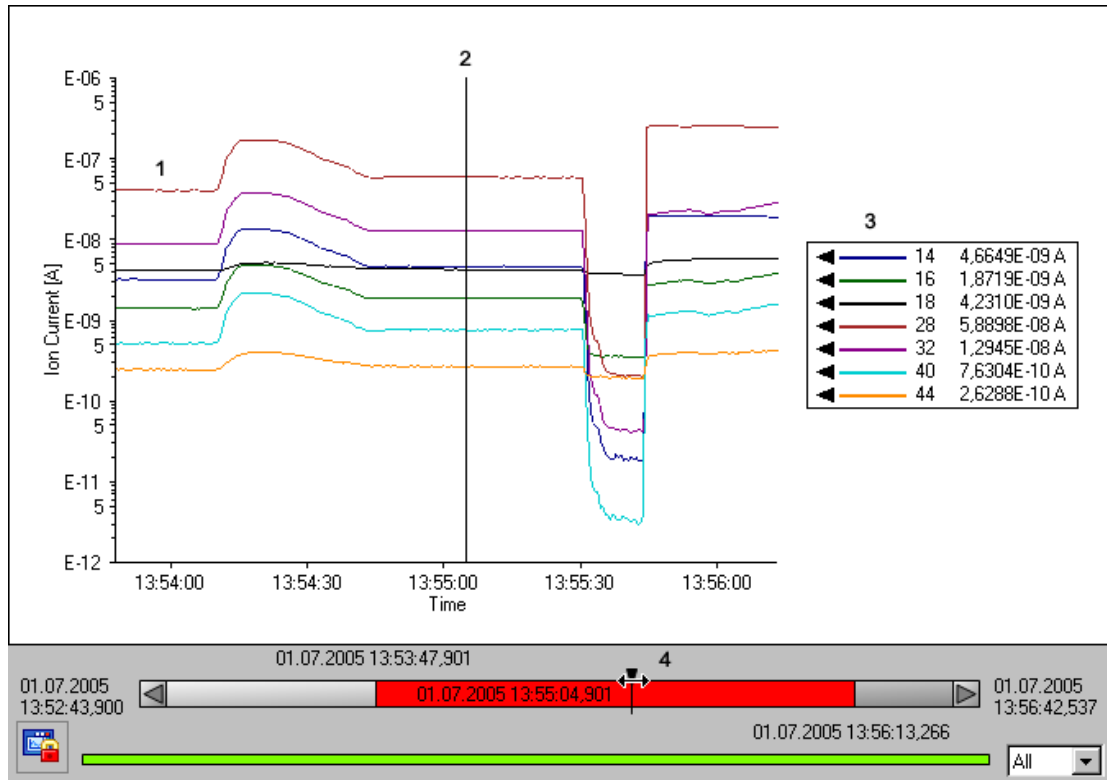


Chart display: Example of a sample measurement (trend)

The measurement data (item 1 in the above figure) are displayed as a function of the time. The chart covers the period of time which is specified by the red scroll bar in the upper navigator bar. The displayed measuring values (item 3) are specified by the cursor position. Please note that the cursor in the red scroll bar (item 4) and the one in the chart (item 2) are synchronized.

"Bar" view


The measuring data are displayed as a bar graph for the point in time specified by the cursor position in the data navigator. The measuring data can only be displayed within the period of time specified by the red scroll bar in the upper navigator bar.

"Table" view

The measuring data are listed as a table for the point in time specified by the cursor position in the data navigator. The measuring data can only be displayed within the period of time specified by the red scroll bar in the upper navigator bar. Please note that the average and the maximum values are still based on the entire time of the measurement.

Exiting QUADERA®

Use one of the following methods to exit QUADERA®:

- In the **File** menu, click **Exit**.
- Press **ALT+F4** (standard method for exiting the currently active Windows application).
- Click the Close symbol  in the upper right corner of the QUADERA® window.
- Call up the context menu for the title bar of the QUADERA® window and click **Close**.

Opening and Managing Measurement Data

Opening an Existing Measurement Project

1. In the **File** menu, click **Open**.
2. Select the directory, the file name and the file type for the required measurement project.
3. Click **Open**.

You may also open an existing measurement project via the Start page.

NOTE:

Continuing the measurement in an existing measurement project that is already saved is not possible. The relevant icons and menu commands are not available.

Recently Used Files

Proceed as follows to open a recently used file:

1. The most recently used files are listed in the lower part of the **File** menu. Click the **More...** button to open a measurement project that is not present in the list.
2. Click the required file in order to open it.

You may also open a recently used file via the Start page.

Exporting a Measurement Project

NOTE:

If you have not selected a section of a Measurement Project then the Export submenu item is disabled.

Exporting

Proceed as follows to export the data of an open measurement project:


1. Select the required section.
2. In the **File** menu, click **Export**.
3. Select the required data format in the submenu:
 - **ASCII** will export the displayed data in the text-only format. You may open and further process these data in any spreadsheet program (e.g. Excel).
4. The "Export Options" window used for selecting measuring data opens up.
 - a. Select the required measurement tasks in the "Measure Tasks" area.
 - b. Select the required data in the "Data Range" area.
 - "All" exports all data of the measurement project,
 - "Selection" exports only the displayed data in the selected section (scan chart, MID chart etc.),
 - "Cycles" exports the selected cycles of the measurement project.
5. Click **OK**. The "ASCII-Export data as" window used for exporting measuring data opens up. Select a suitable name and path and then click **Save**. The measurement project will be exported.

Delimiters, the date and time format, and decimal separators (period and comma) are country specific. These settings can be adjusted in the operating system: Windows Start menu > Control Panel > Date, Time, Language, and Regional Options. The settings for the operating system will also be used by QUADERA®.

Closing a Measurement Project

1. Select the required measurement project window.
2. In the **File** menu, click **Close**.

or

2. Click the Close symbol  in the upper right corner of the measurement project window.

Saving a new measurement project

When closing a new measurement project you are requested to save the measurement project. QUADERA® suggests an automatically generated file name that is based on date/time of the measurement and the template in use.

- Yes: the "Save As" window used for saving measuring data opens up. Select a suitable name and path and then click **Save**. The measurement project will be closed and saved.
Please note: The file extension for measurement projects is *.qmp
- No: the measurement project will be closed without saving the data.
- Cancel: the action is cancelled. You will return to the measurement project without saving the data.

Changing a File Location

In QUADERA®, you can specify the path (file location) for various file types created by the user:

- Templates: Measurement project templates,
- Calibration files: Files containing calibration templates,
- Data files: Files containing measurement projects,
- Exported files: Files containing exported projects.
- Scripting files: Files containing scripting code (Add-ins).

Proceed as follows to change the corresponding paths:

1. In the **Tools** menu, click **Options...** The "Options" window opens up.
2. Click the **File Locations** tab.
3. Select the desired file type.
4. Click **Modify**.
5. The "Browse For Folder" window opens up. Select the desired path and then click **OK**.
6. In the "Options" window, click **OK**.

NOTE:

Click "**Default**" to reset the paths for all file types to the default settings.

Changing the Display of Measurement Projects

Adjusting the Section

You can adjust the display of measuring data in the section, even while a measurement is running. Proceed as follows:

1. Click the section with the right mouse button. The related context menu opens up.
2. Click the required function.

Zooming in Charts

Selection of the zoom area

Use the mouse pointer (displayed as crosshairs in a chart) to mark a rectangle across the required area:

1. Position the crosshairs in one corner of the required rectangle.
2. Press the left mouse button and keep it pressed.
3. Move the cursor to the opposite corner of the rectangle. The zoom area is indicated by a dashed rectangle.
4. Release the left mouse button. The marked area is zoomed in.

NOTE:

For sample measurements, the data navigator displays the time period of the zoomed area of the x-axis (time axis).

Resetting the zoomed area

1. Call up the related context menu.
2. Click **Zoom out** or **Reset Zoom**.

Selecting Curve Colors in Charts

You can select curve colors in charts.

Proceed as follows:

1. Click with the right mouse button into the measuring data legend of the section. The corresponding context menu opens.
2. Click on **Color**.... The "Color" dialog opens.
3. Select the required curve color.
 - Click one of the available basic colors, or
 - Click one of the color fields that has already been defined by you, or
 - Click [Define Custom Colors>>]. A continuous color palette appears and allows you to select a color.
4. Click [OK] to confirm the selection.

For a more detailed description of the "Color" dialog box, please refer to the Windows operating system help.

Defining the Line Thickness in Charts

You can change the line thickness of curves in charts.

Proceed as follows:

1. In the **Tools** menu, click **Options...** The "Options" dialog opens.
2. Click the **Display** tab.
3. Enable the "Smooth Chart Lines" checkbox to smooth the displayed lines in charts.
4. Use the spin buttons to increase and decrease the line thickness.

The settings are applied to the charts for all measurement projects.

Splitting Up the Working Area

You can split up the working area into several sections, i.e. you can add new sections.

Toolbox

Proceed as follows:

1. Select the required working area.
2. Open the corresponding toolbox.
3. Drag the required tool ("Split") onto the working area (drag&drop). The section is split up according to the selected tool.

Deleting a Section

NOTE:

Measurement data remain stored when a section is deleted.

You can remove sections of the working area, i.e. you can delete a section.

Toolbox

Proceed as follows:

1. Open the corresponding toolbox.
2. Drag the **Remove Section** tool onto the required section (drag&drop).
3. You are asked to confirm the deletion of the section. Click **OK**.

The section is deleted and the working area is simplified.

Creating a New Working Area

You can create a new working area in a measurement project. This allows you to display the measurement tasks of a measurement project in different ways according to your requirements (e.g. different combinations of measurement tasks, or the representation as a curve and a bar graph).

Toolbox

Proceed as follows:

1. Select the required measurement project.
2. Open the corresponding toolbox.
3. Drag the **Add Working Area** tool onto the working area (drag&drop). A new tab labeled "New WorkingArea" appears in the working area selection, and the new working area is displayed.
4. Use the context menu "Frame of the section" to rename the new working area as desired.

Deleting a Working Area

NOTE:

Measurement data remain stored when a working area is deleted.

You can delete working areas in a measurement project.

Toolbox

Proceed as follows:

1. Select the required measurement project.
2. Open the corresponding toolbox.
3. Drag the **Remove Working Area** tool onto the working area (drag&drop).
4. You are asked to confirm the deletion of the working area. Click **OK**.

The working area is deleted.

Freezing the Display

You can freeze the display while a measurement is running. This will allow you e.g. to scroll through a measurement or to zoom an area.

Proceed as follows:

1. Click on the measuring data display in the section with the right mouse button. The related context menu opens up.
2. Click **Hold**:
 - The checkmark indicates that the function is enabled, i.e. the display is now frozen.
 - The function is disabled if the checkmark is not shown.

or

1. Click on the "Hold mode" icon in the data navigator. Note that the icon is only displayed when the data navigator is shown.

NOTE:

If you are zooming an area or moving the cursor, the "Hold" function will be switched on automatically, i.e. the display will freeze.

Managing and Arranging Windows

Displaying Windows

QUADERA® can manage several windows at a time. Individual windows can be handled as usual under the Windows operating system (close, move, resize, etc.). You may also use the title bar context menu for the respective window. In addition, the following options are available:

- Show all windows
- Close all windows
- Switch between windows
- Arrange icons

Showing all windows:

- In the **Window** menu, click **Cascade**. This will arrange all open windows in an overlapping manner.
- In the **Window** menu, click **Tile Horizontally**. This will arrange all open windows as horizontal tiles (one below the other).
- In the **Window** menu, click **Tile Vertically**. This will arrange all open windows as vertical tiles (side by side).
- In the **Window** menu, click **Minimize All Windows**. This will minimize all open windows.

Closing all windows:

- In the **Window** menu, click **Close All Windows**. This will close all open windows.

Switching between windows:

1. Open the **Window** menu. A list of all open measurement projects is displayed at the bottom of the pulldown menu.
2. Click the required measurement project in order to move the related window to the front.

When switching to another measurement project, the device status display is always updated. This means that the status of the device belonging to the current measurement project is displayed.

Arranging icons:

- In the **Window** menu, click **Arrange Icons**. This will arrange all icons.

Showing and Hiding Docker Windows

You can show and hide docker windows in the **View** menu.

- Enable the docker window if you want it to be shown,
- Disable the docker window if you want it to be hidden.

Event view

In the **View** menu, click the **Event View** element to show and hide the event view.

Device status

In the **View** menu, click the **Device Status** element to show and hide the device status.

Toolbox

In the **View** menu, click the **Toolbox** element to show and hide the toolbox.

Calling Device Specific Functions

Configuring the Device Connection

The device connection is automatically configured. One simulator per Device type is present (if licensed); other mass spectrometers can be added using '**Search**' in '**Device>>Device Setup**'.

Starting and Stopping the Measurement

NOTE:


New or modified parameters for the measurement task are accepted from the device only after the measurement has been restarted. Ion source parameters affect the device immediately, i.e. as soon as the device is connected with QUADERA®.

Starting the measurement

1. In the device status view, check that the filament and SEM are on. The corresponding icons and tooltips indicate the current status. If required, switch the filament and the SEM on.
When the filament and the SEM are switched off and you want to start the measurement a requester appears automatically. It queries if the corresponding component is to be switched on or not.
2. In the **Device** menu, click **Run**. The connection to the device is automatically established and then the current recipe is started. The checkbox indicates that the measurement is running (checkmark).

or




2. In the device status view, click the "Start" icon . The connection to the device is automatically established and then the current recipe is started. The "Start" icon appears in gray thus indicating a running measurement. The "Stop" icon becomes available.

Stopping the measurement

1. In the **Device** menu, click **Run**. The measurement is being stopped. The checkbox indicates that the measurement has been stopped (no checkmark).

or




1. In the device status view, click the "Stop" icon . The measurement is being stopped. The "Stop" icon appears in gray thus indicating that the measurement is stopped. The "Start" icon becomes available.


Disconnecting From the Device

Disconnecting

1. In the **Device** menu, click **Connect**. The checkbox indicates that the device is no longer connected (no checkmark).

or

1. In the device status view, click the "Connected" icon . After the

connection has been cut the icon toggles to the "Disconnected" icon .

NOTE:

A requester appears if you disconnect the device while the measurement is running:

- Click "Yes" if you want to disconnect the device. The measurement will be stopped.
- Click "No", if you want to continue the measurement. The device will not be disconnected.

Connecting With the Device


NOTE:

New or modified parameters for the measurement task are accepted from the device only after the measurement has been restarted. Ion source parameters affect the device immediately, i.e. as soon as the device is connected with QUADERA®.

Start Page

- Select the desired device. You can choose between a real device and a simulator.

Connecting

- In the **Device** menu, click **Connect**. The checkbox indicates that the device is connected (checkmark), or
- In the device status view, click the "Disconnected" icon . After the connection has been established the icon toggles to the "Connected" icon



Simulation Mode

QUADERA® allows you to simulate the operation of a mass spectrometer. This doesn't mean that a simulation is being performed in the real device; instead, a simulation software is used. By default, the simulation software is installed together with QUADERA®. The simulator is running on the same PC as QUADERA®. The local simulation mode is e.g. helpful for getting familiar with the software.

To use the simulator, select it on the 'Start Page' and use it as you would a real device.

NOTE:

The simulation in the real device is defined via the basic device settings of the device status view ("Device Configuration View" icon). In contrast, using the simulation software (local simulation on the PC) does not require a real device.

Calibration

Calibration Projects

In QUADERA®, devices are calibrated by using calibration projects, which are based on normal measurement projects. Calibration projects are called via the start page.

A calibration project contains the usual views of a measurement project:

- One recipe,
- Working areas for operation and visualization.

You can modify recipe parameters directly in the recipe. The parameters that are relevant for the calibration project are linked to editing fields in the working area. Thus, you can change these parameters directly in the working area.

QUADERA® provides basic templates for each calibration project, such as gas specific calibration and background determination. These templates are intended to create user specific calibration project templates, for ab initio calibration projects.

Saving the measurement data of a calibration procedure is usually not required. However, saving the calibration project as a template may be useful for future applications (menu **File** > **Save as Template...**). Example: creating GSC measurement projects.

NOTE:

For a written documentation of your calibration projects you can capture screens of the QUADERA® user interface.

Tuning the Ion Source

Tuning the Ion Source

Consider one or two peaks of a scan-analog measurement to tune the ion source (ion source optimization). Use the recipe editor to change the recipe parameters defined in the calibration project for the ion source. Typically, one or more masses are scanned.

The calibration project allows you to optimize the performance of the ion source. The scans will be recorded when you start the calibration project. The currently set ion source parameters are used. They are displayed in the working area. Tune the ion source while the measurement is running; optimize the peak shape and intensity by changing the ion source parameters. Changed parameters are forwarded from the calibration project to the device and accepted instantly.

Optimizing the Ion Source

1. Open the start page: In the **View** menu, click **Show Start Page**.
2. Click on the icon for the required device.
3. Create a new calibration project: In the "Calibration and Tuning" list, double-click **Ion Source Tuning.qmt**. This way you create a new calibration project based on the selected template.
4. The new measurement project window appears. The working area displays the calibration project.
 - Edit the recipe according to your needs (if necessary): Click the corresponding tab in the working area selection.
 - Display the measuring data: Click the corresponding tab in the working area selection.

NOTE:

You can start the measurement regardless whether the recipe editor or the working area has been selected.

5. Start the measurement: In the device status view, click on the "Start" icon. The connection to the device is automatically established. The device now receives the parameters for the current measurement task. You can adjust the chart layout while the measurement is running.
6. Optimize the peak shape and intensity: Change the ion source parameters in the section of the calibration project during the measurement ("Ion Source" editor). Changed parameters are accepted by the device instantly. You will find the procedures to optimize the ion source potentials for the QMG700 with QMA400/410/430 in the operating instructions BG 805983 BD/E. Procedures to optimize the specific ion source types for the QMG220:
 - Crossbeam Ion Source
 - Grid Ion Source
 - SPM Ion Source
 - Open High Sensitivity Ion Source
 - Gastight High Sensitivity Ion Source
7. Stop the measurement: In the device status view, click on the "Stop" icon.
8. Close and save the measurement project. In the **File** menu, click **Close**. You are requested if you want to save the measurement project. QUADERA® suggests an automatically generated file name that is based on date/time of the measurement and the used template.
 - Yes: the "Save As" window used for saving measuring data opens up. Select a suitable name and path and then click **Save**. The measurement project will be saved and closed. Please note: The file extension for measurement projects is *.qmp
 - No (recommended option): the measurement project will be closed without saving the data.

- Cancel: the action is cancelled. You will return to the measurement project without saving the data.

NOTE: The filament Ion Source can be degassed from the Device Configuration window.

Ion Source Parameters

The "Ion Source" editor in the calibration project displays the parameters for tuning the ion source. Modify the parameters directly in this editor. The device applies modified parameters instantly.

- Ion source parameters for QMG220
- Ion source parameters for QMG700

A separate parameter set is stored for each ion source type and filament. The QMG220 additionally provides 4 parameter sets per ion source type, containing ion source voltages ("Active Set").

Image of "Ion Source" editor (example)

Ion source parameters for QMG220

Parameter	Range	Description
• Ion Source Type	(not editable)	Use the "Device Configuration" window to select the ion source type.
• Filament Number	Dropdown list	Filament selection. The number of available filaments depends on the ion source type.
• Active Set	Dropdown list	Select the ion source voltages parameter set, which contains each one data set for the various filament configurations.
• Emission Current	Number > 0	Filament emission current. This parameter is applied to the filament that is selected under "Filament Number".
• Protection Current	Number > 0	Maximum filament current, used to protect the filament. This parameter is applied to the filament that is selected under "Filament Number".
• RF-Polarity	Dropdown list	Switch the polarity of the rod system for separating ions by the m/e-ratio.
• Ion Reference	Any number	Ion source voltages.
• Cathode		These parameters are applied to the filament and the ion source

- Focus
 - Field Axis
 - Extraction
 - Inner Deflection
 - Outer Deflection
 - Wehnelt
- type that is selected under "Filament Number" and "Ion Source Type", respectively. The available parameters depend on the used ion source. For detailed information, please refer to the operating instructions of the QMG and the used ion source.
- Procedures to optimize the specific ion source types:
- Crossbeam Ion Source
 - Grid Ion Source
 - SPM Ion Source
 - Open High Sensitivity Ion Source
 - Gastight High Sensitivity Ion Source

Ion source parameters for QMG700

Parameter	Range	Description
<ul style="list-style-type: none"> • Ion Source Type 	(not editable)	Use the "Device Configuration" window to select the ion source type.
<ul style="list-style-type: none"> • Filament Number 	Dropdown list	Filament selection. The number of available filaments depends on the ion source type.
<ul style="list-style-type: none"> • Emission Current 	Number > 0	Filament emission current. This parameter is applied to the filament that is selected under "Filament Number".
<ul style="list-style-type: none"> • Filament Protection Current 	Number > 0	Maximum filament current, used to protect the filament. This parameter is applied to the filament that is selected under "Filament Number".
<ul style="list-style-type: none"> • Ion Reference • Cathode • Focus • Field Axis • Extraction 	Any number	Ion source voltages. These parameters are applied to the filament and the ion source type that is selected under "Filament Number" and "Ion Source Type", respectively. The available parameters depend on the used ion source. For detailed

QUADERA HTML Help

- Inner Deflection
- Outer Deflection
- Wehnelt

information, please refer to the operating instructions of the QMG and the used ion source.

You will find the procedures to optimize the ion source potentials for the QMG700 with QMA400/410/430 in the operating instructions BG 805983 BD/E.

Ion Source Editor	
Ion Source Type	Crossbeam
Active Set	Set1
Emission Current	1,00
Filament Number	No1
Protection Current	4,40
RF-Polarity	pos
Ion Reference	105,00
Cathode	0,00
Focus	-6,00
Field Axis	-7,00
Extraction	-50,00

Crossbeam Ion Source

This topic applies to the QMG220.

Proceed as follows to optimize the crossbeam ion source:

1. Select the filament and operate it with 1 mA emission current for approximately half an hour. The message "Emission Error" appears repeatedly: start with reduced emission current and increase it slowly.

Default settings:

- Emission Current: 1 mA
- Protection Current: 4.0 A
- RF-Polarity: pos
- Ion Reference: 150 V
- Cathode: -70 V
- Focus: -5 V
- Field Axis: -10 V
- Extract: -50 V

3. Wait until the pressure reaches $< 10^{-7}$ mbar and the residual gas spectrum remains stable.
4. Introduce a test gas, such as air, into the recipient for a pressure of 10^{-6} mbar. Otherwise, use the residual gas to perform the optimization procedure.
5. Repeatedly record spectra of the relevant peaks (e.g. 25...34 m/e). Observe intensity, resolution, and peak shape.
6. Optimize the ion source voltages:
 - a. Check which "RF-Polarity" ("pos" or "neg") results in the better peak shape and select this polarity.
 - b. Optimize "Cathode" for best sensitivity.
 - c. Adjust "Field Axis" for useful resolution and peak shape.
 - d. Optimize "Extract" and "Focus" alternately for maximum peak height.

The ion source is optimized.

Grid Ion Source

This topic applies to the QMG220.

Proceed as follows to optimize the grid ion source:

1. Select the filament and operate it with 2 mA emission current for approximately half an hour. The message "Emission Error" appears repeatedly: start with reduced emission current and increase it slowly.

Default settings:

- Emission Current: 2 mA
- Protection Current: 4.0 A
- RF-Polarity: pos
- Ion Reference: 150 V
- Cathode: -90 V
- Field Axis: -12 V

Vary the "Field Axis" potential to optimize sensitivity, peak shape, and resolution.

3. Wait until the pressure reaches $< 10^{-8}$ mbar and the residual gas spectrum remains stable.
4. Repeatedly record spectra of the relevant peaks (e.g. 25...34 m/e). Observe intensity, resolution, and peak shape.
5. Optimize the ion source voltages:
 - a. Check which "RF-Polarity" ("pos" or "neg") results in the better peak shape and select this polarity.
 - b. Optimize "Cathode" for best sensitivity.
 - c. Adjust "Field Axis" for useful resolution and peak shape.

The ion source is optimized.

SPM Ion Source

This topic applies to the QMG220.

Proceed as follows to optimize the SPM ion source:

1. Select the filament and operate it with 1 mA emission current for approximately half an hour. The message "Emission Error" appears repeatedly: start with reduced emission current and increase it slowly.
2. Introduce a process gas, such as argon, into the process chamber for a pressure of 10^{-3} ... 10^{-2} mbar.
3. Repeatedly record spectra of the relevant peaks (e.g. argon 32...41 m/e). Observe intensity, resolution, and peak shape.

Default settings:

- Emission Current: 1 mA
- Protection Current: 3.5 mA
- Ion Reference: 105 V
- Cathode: -40.0 V
- Focus: -2.0 V
- Field Axis: -2.0 V
- Extract: -60 V

4. Optimize the ion source voltages:
 - a. Set "Field Axis" to -5 V.
 - b. Decrease "Field Axis" for useful resolution and peak shape.

The ion source is optimized.

Open High Sensitivity Ion Source

This topic applies to the QMG220.

Proceed as follows to optimize the open high sensitivity ion source:

1. Select the filament and operate it with 2 mA emission current for approximately half an hour ("Protection Current" at 3.5 A). The message "Emission Error" appears repeatedly: start with reduced emission current and increase it slowly.

Default settings:

- Emission Current: 2 mA
- Protection Current: 3.5 A
- RF-Polarity: pos
- Ion Reference: 150 V
- Cathode: -75 V
- Focus: -5 V
- Field Axis: -7 V
- Extract: -50 V

3. Wait until the pressure reaches $< 10^{-7}$ mbar and the residual gas spectrum remains stable.
4. Introduce a test gas, such as air, into the recipient for a pressure of 10^{-6} mbar. Otherwise, use the residual gas to perform the optimization procedure.
5. Repeatedly record spectra of the relevant peaks (e.g. 25...34 m/e). Observe intensity, resolution, and peak shape.
6. Optimize the ion source voltages:
 - a. Check which "RF-Polarity" ("pos" or "neg") results in the better peak shape and select this polarity.
 - b. Optimize "Cathode" for best sensitivity.
 - c. Adjust "Field Axis" for useful resolution and peak shape.
 - d. Optimize "Extract" and "Focus" alternately for maximum peak height.

The ion source is optimized.

Gastight High Sensitivity Ion Source

This topic applies to the QMG220.

Proceed as follows to optimize the gastight high sensitivity ion source:

- Using air as test gas,
- Using argon and avoiding double ionization

Using air if no specific test gas is available

1. Select the filament and operate it with 1 mA emission current for approximately half an hour ("Protection Current" at 3.5 A). The message "Emission Error" appears repeatedly: start with reduced emission current and increase it slowly.

Default settings for air as test gas:

- Emission Current: 1 mA
- Protection Current: 3.5 A
- RF-Polarity: pos
- Ion Reference: 150 V
- Cathode: -60 V
- Focus: -5 V
- Field Axis: -7 V
- Extract: -50 V

2. Repeatedly record spectra of the relevant peaks (e.g. 25...34 m/e). Observe intensity, resolution, and peak shape.

3. Optimize the ion source voltages:

- a. Check which "RF-Polarity" ("pos" or "neg") results in the better peak shape and select this polarity.

- b. Optimize "Cathode" for best sensitivity.
- c. Adjust "Field Axis" for useful resolution and peak shape.
- d. Optimize "Extract" and "Focus" alternately for maximum peak height.

The ion source is optimized.

Using argon and avoiding double ionization

1. Select the filament and operate it with 1 mA emission current for approximately half an hour ("Protection Current" at 3.5 A). When the message "Emission Error" appears repeatedly start with reduced emission current and increase it slowly.

Default settings for argon
as test gas:

- Emission Current: 1 mA
- Protection Current: 3.5 A
- RF-Polarity: pos
- Ion Reference: 105 V
- Cathode: -40 V
- Focus: -5 V
- Field Axis: -6 V
- Extract: -50 V

2. Repeatedly record spectra of the relevant peaks (e.g. 35...42 m/e). Observe intensity, resolution, and peak shape.

3. Optimize the ion source voltages:

- a. Check which "RF-Polarity" ("pos" or "neg") results in the better peak shape and select this polarity.
- b. Leave "Cathode" at -40 V to avoid double ionization.
- c. Adjust "Field Axis" for useful resolution and peak shape.

- d. Optimize "Extract" and "Focus" alternately for maximum peak height.

The ion source is optimized.

Tuning the Mass Scale

Calibrating the Mass Scale

Basics

Gas components are represented by integer mass numbers. Typically, the measuring apparatus causes small deviations between the nominal mass number and the actual position of the peak maximum. The correct position of the peak maxima is usually close to theoretical value, e.g. at 13.95 instead of 14.00. However, an exact measurement requires measuring the peak maximum. To achieve best accuracy in measurements, the exact position of the peak maxima has to be determined by calibrating the mass scale.

Procedure

QUADERA® uses two steps to calibrate the mass scale:

- Coarse tuning:
Two parameters are used to shift and to shrink or stretch the mass scale. This coarse tuning will be applied to all measurements.
- Fine tuning:
The fine tuning is based on the coarse tuning and compensates nonlinearity of the mass scale by manually entering corrected mass values. This fine tuning is applied to sample measurements and scan-stair measurements, and also to scan-analog measurements with the QMG700.

The Fine Tuning process is a manual process.

A **Mass Scale Adjust** template is provided that automates the determination of measured mass numbers. This template can be configured through the Recipe Editor; the decision to save or discard Mass Scale Tune Entries is still left to the user.

Mass Scale Adjust uses the following controls:

Update Mass List – Adds new masses from the Recipe into the Mass Adjust list. In order to update the Mass Adjust list, masses must first be entered into the Recipe as Measurement Tasks.

Remove Mass – Removes a selected Mass from the Mass Adjust list. This action has no effect on the Masses (Measurement Tasks) in the Recipe.

Apply to Mass Scale Table – Downloads the changes made in Mass Scale Adjust to the device Mass Scale Table. This action commits and saves the changes determined by QUADERA (and the device) into the device.

Reset Mass Scale Table – Resets all Actual Masses in the Mass Adjust list to their respective Reference Mass.

State column – The following states can occur when running Mass Scale Adjust:

- Ok: The calibration has been successfully performed; the exact mass numbers are shown in the column Actual Mass.
- Mass number too low: The entered mass number is too far to the left of the peak (i.e. too low in AMU).
- Mass number too high: The entered mass number is too far to the right of the peak (i.e. too high in AMU).
- Peak Intensity below threshold: Intensity lower than the level defined by the Threshold parameter.
- Peak Intensity too high: Intensity equal to or higher than full scale range.
- Peak width too narrow: The peak is too narrow to determine a maximum.
- Mass number too low; intensity tail too high: Intensity is too constant to determine a maximum.

Two scan analog measurements in various mass ranges are used for tuning of the mass scale. The recipe parameters are defined in the calibration project for the mass scale. Use the recipe editor to change the parameters. Normally, scanned masses range from one up to many masses.

NOTE:

It is preferred that the two scans cover a mass range as wide as possible. One peak should appear at a very low mass number, another one at a very high mass number.

Scan recording begins when the calibration project is started. The currently set mass scale parameters are applied and displayed in the working area. Perform the tuning procedure during the course of the measurement: Modify the parameters to adjust the peak positions to the nominal mass numbers. You can observe the effect of modified parameters during the next cycle and iteratively tune the mass scale.

Coarse Tuning of the Mass Scale

1. Feed a suitable calibration gas into the vacuum chamber. Use air if special calibration gases are not available.
2. Open the start page: In the **View** menu, click **Show Start Page**.
3. Click on the icon for the required device.
4. Only for QMG700: Reset the fine tuning data points before starting the coarse tuning procedure of the mass scale. Fine tuning is applied to scan analog measurements and will affect the coarse tuning.
5. Create a new calibration project: In the "Calibration and Tuning" list, double-click e.g. **Mass Scale Tuning (Coarse).qmt**. This way you create a new calibration project based on the selected template. You can modify it according to your needs.
6. The new measurement project window appears. The working area displays the calibration project.
 - Edit the recipe according to your needs (if necessary): Click the corresponding tab in the working area selection,
 - Display the measuring data: Click the corresponding tab in the working area selection.

NOTE:

You can start the measurement regardless whether the recipe editor or the working area has been selected.

7. Start the measurement: In the device status view, click on the "Start" icon. The connection to the device is automatically established. The device now receives the parameters for the current measurement task. You can adjust the chart layout while the measurement is running.
 8. Adjust the actual peak positions to the nominal mass numbers: change the parameters in the section of the calibration project ("Mass Scale Tuning" editor) while the measurement is running. You can observe the effect of modified parameters during the next measurement task and iteratively tune the mass scale.
 - "Mass Scale Offset" shifts the mass scale,
 - "Mass Scale Slope" shrinks and stretches the mass scale.
8. Perform a fine tuning of the mass scale (if required). Otherwise, reset the fine tuning values to the default values.
 9. Stop the measurement: In the device status view, click on the "Stop" icon.
 10. Close and save the measurement project. In the **File** menu, click **Close**. You are requested if you want to save the measurement project.

QUADERA HTML Help

QUADERA® suggests an automatically generated file name that is based on date/time of the measurement and the used template.

- Yes: the "Save As" window used for saving measuring data opens up. Select a suitable name and path and then click **Save**. The measurement project will be saved and closed.

Please note: The file extension for measurement projects is *.qmp

- No (recommended option): the measurement project will be closed without saving the data.
- Cancel: the action is cancelled. You will return to the measurement project without saving the data.

NOTE:

The coarse tuning of the mass scale will be applied to all measurements.

Fine Tuning of the Mass Scale

NOTE:

Perform the fine tuning of the mass scale exclusively within a coarse tuning procedure.

1. Feed a suitable calibration gas into the vacuum chamber. Use air if special calibration gases are not available.
2. Open the start page: In the **View** menu, click **Show Start Page**.
3. Click on the icon for the required device.
4. Create a new calibration project: In the "Calibration and Tuning" list, double-click e.g. **Mass Scale Tuning (Fine).qmt**. This way you create a new calibration project based on the selected template. You can modify it according to your needs.
5. The new measurement project window appears. The working area displays the calibration project.
 - Edit the recipe according to your needs (if necessary): Click the corresponding tab in the working area selection.
 - Display the measuring data: Click the corresponding tab in the working area selection.

NOTE:

You can start the measurement regardless whether the recipe editor or the working area has been selected.

6. Start the measurement: In the device status view, click on the "Start" icon. The connection to the device is automatically established. The device now receives the parameters for the current measurement task. You can adjust the chart layout while the measurement is running.
 7. Define the data points for the linear interpolation of the mass scale ("Mass Scale Tune Fine" editor):
 - a. Enter the nominal mass number in the "Nominal Mass" fields.
 - b. Enter the measured mass number in the "Actual Mass" fields (use the cursor to locate peak maximum).
 8. Adding and deleting data points:
 - Press ENTER when you have input the mass numbers. This way you add a row for a new data point.
 - Use the context menu of the "Mass Scale Tune Fine" editor to delete data points.
 - Delete all rows in the editor if there is no need for mass scale fine tuning: Click **Delete Mass Scale Tune Fine Entries**.

9. Stop the measurement: In the device status view, click on the "Stop" icon.

10. Close and save the measurement project. In the **File** menu, click **Close**. You are requested if you want to save the measurement project. QUADERA® suggests an automatically generated file name that is based on date/time of the measurement and the used template.

- Yes: the "Save As" window used for saving measuring data opens up. Select a suitable name and path and then click **Save**. The measurement project will be saved and closed.
Please note: The file extension for measurement projects is *.qmp
- No (recommended option): the measurement project will be closed without saving the data.
- Cancel: the action is cancelled. You will return to the measurement project without saving the data.

NOTE:

The fine tuning of the mass scale will be applied to MID/MCD measurements and to scan-stair measurements, and also to scan-analog measurements with the QMG700.

NOTE: A Mass Scale Adjust template is provided that automates the determination of measured mass numbers. This template can be configured through the Recipe Editor; the decision to save or discard Mass Scale Tune Entries is still left to the user.

Parameters for Coarse Tuning


Two parameters are used for coarse tuning, to shift and to shrink or stretch the mass scale. This way you can match the actual peaks with the nominal mass numbers.

The "Mass Scale Tune Coarse" editor in the calibration project displays the parameters for coarse tuning of the mass scale. Modified parameters are forwarded to the device and take effect in the next measurement cycle.

Image of "Mass Scale Tune Coarse" editor" (example)

Parameter	Range	Description
• Mass Scale Offset	-0.12 < Offset < 0.12	Shift the mass scale to the left and right for negative and positive values, respectively.
• Mass Scale Slope	0.985 < Slope < 1.015	Shrink and stretch the mass scale for values < 1.000 and > 1.000, respectively.

QUADERA HTML Help

Mass Scale Offset	0.000	
Mass Scale Slope	0.996	

Parameters for Fine Tuning

The fine tuning is based on the coarse tuning and compensates nonlinearity of the mass scale. You have to perform the fine tuning when the coarse tuning has been changed. Modified parameters are forwarded to the device and take effect in the next measurement cycle.

Data points on the mass scale have to be input for the fine tuning. These points are used for linear interpolation of mass numbers located in between. The "Mass Scale Tune Fine" editor lists the data points in a table. Use the context menu of this editor to delete data points.

Image of "Mass Scale Tune Fine" editor (example)

Parameter	Range	Description
<ul style="list-style-type: none"> Nominal Mass 	Integer number	Nominal mass number: Data point for the interpolation. <ul style="list-style-type: none"> The listed values are sorted by increasing nominal mass number, Only one input is allowed per nominal mass.
<ul style="list-style-type: none"> Actual Mass 	+/- 0.5 amu around the nominal mass number	Measured mass number
<ul style="list-style-type: none"> Delete Mass Scale Tune Fine Entries 	Button	Delete the data points input by the user in the "Mass Scale Tune Fine" editor.

Context menu for the "Mass Scale Tune Fine" editor

In this context menu the following commands are available:

- Delete selected rows:** Delete the selected rows, i.e. remove the data points.

QUADERA HTML Help

	Nominal Mass	Actual Mass
▶	12	12.0
	18	18.1
	28	28.0
	32	32.0
	44	43.9

Offset

Offset

Basics

The offset is caused by a drift of the measuring amplifier and can be compensated by a correction measurement. The measured intensity will be applied to future measurement projects by subtracting it from the results of the corresponding measurement tasks. You cannot switch on and off the offset values for saved data.

Procedure

The measurement of the offset is performed by the device automatically. However, there is no real measurement. Instead, the offset of the electronic circuit of the measuring amplifier is determined for each measuring range at a defined mass number. The values are automatically stored in the device and will remain after the power has been cut.

Determining the Offset

NOTE:

Determine the offset for the electrometer preamplifier and detector, which you intend to use in the subsequent measurement:

- **QMG220: one electrometer preamplifier is used with both detectors (if installed), i.e. there is only one set of offset values,**
- **QMG700: individual electrometer preamplifiers are used with both detectors (if installed), i.e. there are two different sets of offset values.**

1. Open the start page: In the **View** menu, click **Show Start Page**.
2. Click on the icon for the required device.
3. Create a new calibration project: In the "Calibration and Tuning" list, double-click e.g. **Offset Calibration.qmt**. This way you create a new calibration project based on the selected template. You can modify it according to your needs.
4. The new measurement project window appears. The working area displays the calibration project.
5. Only QMG700:
Select the detector corresponding to the measuring amplifier ("Electrometer Preamplifier") whose offset is to be determined:
 - Faraday,
 - SEM.
6. Edit the mass ("Offset Mass") for the offset measurement.
7. Start the measurement: In the device status view, click on the "Start" icon. The connection to the device is automatically established. The device now receives the parameters for the current measurement task. The measurement runs automatically and should take about 10...15 s.
8. QUADERA® calculates the necessary offset values. The values are automatically stored for the individual measuring ranges of the amplifier and applied to future measurement projects.
9. Close and save the measurement project. In the **File** menu, click **Close**. You are requested if you want to save the measurement project. QUADERA® suggests an automatically generated file name that is based on date/time of the measurement and the used template.
 - Yes: the "Save As" window used for saving measuring data opens up. Select a suitable name and path and then click **Save**. The measurement project will be saved and closed.
Please note: The file extension for measurement projects is *.qmp
 - No (recommended option): the measurement project will be closed without saving the data.

- Cancel: the action is cancelled. You will return to the measurement project without saving the data.

Offset Parameters

The calibration project displays the parameters required to determine the offset. Modified parameters are forwarded to the device and take effect in the next measurement task.

Offset parameters QMG220

Parameter	Range	Description
<ul style="list-style-type: none"> E-05 ... E-12 	(not editable)	<p>Offset value for the corresponding measuring range of the detector.</p> <p>The device automatically determines the values listed in the corresponding table.</p> <p>See also recipe parameter "Amplifier Range".</p>
<ul style="list-style-type: none"> Offset Mass 	$0 \leq \text{value} \leq \text{MaxRange}$	Mass for the offset measurement.
<ul style="list-style-type: none"> Delete Offset Entries 	Button	Deletes the offset values for the detector.

Offset parameters QMG700

Parameter	Range	Description
<ul style="list-style-type: none"> E-05 ... E-12 	(not editable)	<p>Offset value for the corresponding measuring range of the selected detector.</p> <p>The device automatically determines the values listed in the corresponding table.</p> <p>See also recipe parameter "Amplifier Range".</p>
<ul style="list-style-type: none"> Electrometer Preamplifier 	Dropdown list	<p>Detector type for the offset determination.</p> <ul style="list-style-type: none"> Faraday, SEM
<ul style="list-style-type: none"> Offset Mass 	$0 \leq \text{value} \leq \text{MaxRange}$	Mass for the offset measurement.

- Delete Offset Entries

Button

Deletes the offset values for the detector that is selected in "Electrometer Preamplifier".

Tuning the RF Generator

Tuning the RF Generator

Basics

The high frequency voltage of the RF generator (QMH, or RF22x for QMG220, see device settings) is applied to the rod pairs of the QMG to separate ions. The output resonant circuit of the generator has to be matched to the QMG rod system in the following cases:

- when commissioning the device,
- problems appear when masses near the upper mass scale limit are measured.

Procedure

Tuning the RF generator requires to turn the tuning screw. The calibration project in QUADERA® is used to display and check the tuning voltage.

NOTE:

Use the device specific instructions (OEM manual) when tuning the RF generator.

- Tuning the RF generator for the QMG220,
- Tuning the RF generator for the QMG700.

Minimizing the Tuning Voltage (QMG220)

This topic applies to the QMG220.

NOTE:

Use the device specific instructions (OEM manual) when tuning the RF generator.

1. Open the start page: In the **View** menu, click **Show Start Page**.
2. Click on the icon for the required device.
3. Create a new calibration project: In the "Calibration and Tuning" list, double-click **RF Tuning.qmt** or **Tune Data.qmt**. This way you create a new calibration project based on the selected template.

NOTE: The mass settings of Tune Data.qmt should be adjusted before tuning the RF generator.

1. The new measurement project window appears. The working area displays the calibration project. Note:
 - No recipe is assigned to this calibration project (**RF Tuning.qmt**). Thus, no user specific adaptation is available.
 - An actual measurement is not performed, i.e. you can not start and stop the measurement.
5. Proceed as follows to tune the output resonant circuit of the generator:
 - Observe the signal bar in the working area. It displays the actual generator tuning voltage. The two drag indicators show the maximum and minimum achieved voltage.
 - Use the **Reset Arrows** command of the context menu "Chart" to reset the two drag indicators.
 - Not available in Tune Data.qmt.
 - Adjust the tuning screw of the generator to minimize the tuning voltage. Refer to the OEM manual. The tuning voltage should not exceed half of the maximum signal.

NOTE:

Do not damage the tuning screw of the generator. Never tighten or remove the tuning screw.

6. Close and save the measurement project. In the **File** menu, click **Close**. You are requested if you want to save the measurement project. QUADERA® suggests an automatically generated file name that is based on date/time of the measurement and the used template.
 - Yes: the "Save As" window used for saving measuring data opens up. Select a suitable name and path and then click **Save**. The measurement project will be saved and closed.
Please note: The file extension for measurement projects is *.qmp

QUADERA HTML Help

- No (recommended option): the measurement project will be closed without saving the data.
- Cancel: the action is cancelled. You will return to the measurement project without saving the data.

Extended context menu "Chart"

In the calibration project "RF Tuning" the context menu "Chart" provides an additional command:

- **Reset Arrows** Reset the drag indicators that show the maximum and minimum achieved tuning voltage.

Minimizing the Tuning Voltage (QMG700)

This topic applies to the QMG700.

NOTE:

Use the device specific instructions (OEM manual) when tuning the RF generator.

1. Open the start page: In the **View** menu, click **Show Start Page**.
2. Click on the icon for the required device.
3. Create a new calibration project: In the "Calibration and Tuning" list, double-click **RF Tuning.qmt** or **Tune Data.qmt**. This way you create a new calibration project based on the selected template.
4. The new measurement project window appears. The working area displays the calibration project. Note:
 - No recipe is assigned to this calibration project. Thus, no user specific adaptation is available.
 - An actual measurement is not performed, i.e. you can not start and stop the measurement.
5. The QMH is set to the maximum mass number in **RF Tuning.qmt**. Tune the output resonant circuit as described in the instructions of the RF generator.

NOTE: The mass settings of Tune Data.qmt should be adjusted before tuning the RF generator.

NOTE:

Do not damage the tuning screw of the generator. Never tighten or remove the tuning screw.

6. Close and save the measurement project. In the **File** menu, click **Close**. You are requested if you want to save the measurement project. QUADERA® suggests an automatically generated file name that is based on date/time of the measurement and the used template.
 - Yes: the "Save As" window used for saving measuring data opens up. Select a suitable name and path and then click **Save**. The measurement project will be saved and closed.
Please note: The file extension for measurement projects is *.qmp
 - No (recommended option): the measurement project will be closed without saving the data.
 - Cancel: the action is cancelled. You will return to the measurement project without saving the data.

Background Determination

Background Determination

Basics

The mass spectrometer background is caused by residual gases. These gases are present in every analysis chamber and do not originate from the measuring sample. The background is mainly constant if the measuring apparatus is well conditioned. However, measurement results may be distorted if the background is not considered properly. The background determination identifies the existing residual gases. The detected ion currents are subtracted from subsequent measurement projects. The result will show the true composition of the measuring gas.

Procedure

Residual gases are measured either with the gas inlet closed or by using a zero gas, i.e. a pure gas that is fed into the analysis chamber to reach the same pressure as expected for future measurements. Using a zero gas takes account of adsorption and desorption effects better than pumping down the chamber to final vacuum.

An MID measurement is used to determine the background. The recipe parameters are defined in the corresponding calibration project. Use the recipe editor to change the parameters. You can determine the mass spectrometer background for **each detector type separately** and store the results in the Background Library. The stored values will be used in future MID and MCD measurement projects where they are subtracted from the measured signals.

NOTE:

Always pump down the chamber to final vacuum before performing the background determination, or let in a suitable zero gas. Otherwise, serious measurement errors may result.

Measuring the Background

NOTE:

Before starting the measurement, check the correct calibration of the mass spectrometer components. If a calibration is necessary, perform the following preparatory measurements:

- Calibrate the mass scale,
 - Determine the offset.
1. Feed a suitable zero gas into the vacuum chamber, or pump the chamber down to final vacuum.
 2. Open the start page: In the **View** menu, click **Show Start Page**.
 3. Click on the icon for the required device.
 4. Create a new calibration project: In the "Templates" list, double-click e.g. **Background Determination.qmt**. This way you create a new calibration project based on the selected template. You can modify it according to your needs.
 5. The new measurement project window appears. The working area displays the calibration project.
 - Edit the recipe according to your needs (if necessary): Click the corresponding tab in the working area selection. The measurement tasks must not contain mass numbers where peaks of the zero gas appear.
 - Display the measuring data: Click the corresponding tab in the working area selection.

NOTE:

You can start the measurement regardless whether the recipe editor or the working area has been selected.

6. Start the measurement: In the device status view, click on the "Start" icon. The connection to the device is automatically established. The device now receives the parameters for the current measurement task. The measurement is running automatically.
7. Check the measured values, e.g. display the measuring data in a table.
8. Click **Apply to Background Library** to forward the background measurement to the Background Library. Note:
 - New background measurements (mass numbers) are added to the Background Library,
 - Current measuring values replace existing data sets in the Background Library.
9. Close and save the measurement project. In the **File** menu, click **Close**. You are requested if you want to save the measurement project. QUADERA®

suggests an automatically generated file name that is based on date/time of the measurement and the used template.

- Yes: the "Save As" window used for saving measuring data opens up. Select a suitable name and path and then click **Save**. The measurement project will be saved and closed.
Please note: The file extension for measurement projects is *.qmp
- No (recommended option): the measurement project will be closed without saving the data.
- Cancel: the action is cancelled. You will return to the measurement project without saving the data.

NOTE:

The data sets in the Background Library will be subtracted in MID and MCD measurements. If you wish to skip this subtraction then reset the data sets in the Background Library ("Delete Background Library" button). Background Subtraction can also be disabled, without resetting the Background Library, from the context menu when running a Measurement Project.

Background Library

The Background Library in the section of the calibration project displays the parameters required to determine the background. Changed parameters take effect in the next measurement task.

The Background Library contains the corresponding background data for all measured mass numbers in tabular form. You can use various zero gases and perform consecutive background determinations. The results can be combined in the Background Library (function "Apply to Background Library"). Note that an individual Background Library is created for each installed detector.

Image of background library (example)

Parameter	Range	Description
<ul style="list-style-type: none"> Detector 	Dropdown list	<p>The Background Library is displayed for the selected detector type:</p> <ul style="list-style-type: none"> Faraday: the table for the Faraday detector is displayed. SEM: the table for the SEM detector is displayed. IonCounter (only QMG700): the table for the ion counter is displayed.
<ul style="list-style-type: none"> Mass 	Mass number (not editable)	Mass number for which the background has been determined: applied from the related MID recipe ("Mass" parameter).
<ul style="list-style-type: none"> Intensity 	Measured value	Background intensity at the related mass number: corresponds to the currently measured value for this mass number.
<ul style="list-style-type: none"> Apply to Background Library 	Button	<p>Apply the result of the current background determination to the Background Library for the detector that is selected in the recipe.</p> <p>NOTE:</p> <ul style="list-style-type: none"> New background measurements are added to the Background Library,

- Delete Background Library Button

- Current measuring values replace existing data sets in the Background Library.

Delete all data sets of the Background Library, for all detectors.

NOTE:
"Delete Background Library" deletes the data sets of the Background Library irretrievably. In this case, a new background determination is required for new data sets.

Mass	Intensity
14	2,2100E-11 A
▶ 16	1,5300E-11 A
18	4,8900E-10 A
28	3,8700E-10 A
32	8,4600E-11 A
40	5,9300E-12 A
44	5,9300E-12 A

Gas Specific Calibration

Gas Specific Calibration

NOTE:

Perform the following preparatory measurements before the gas specific calibration:

- **Calibrate the mass scale,**
- **Determine the offset,**
- **Determine the background.**

Basics

An MCD measurement project uses a matrix of calibration factors (analysis matrix) to convert ion currents into gas concentrations. The calibration factors are not universally valid. They have to be quantified by a separate calibration measurement using known gases (calibration gases). Calibration gases are selected according to the components in the measurement project whose concentrations are to be measured.

NOTE:

Gas mixtures that contain components with overlapping masses are not suited for use as calibration gas. The same mass number must not be assigned to several components.

Procedure

One MID measurement project is created per calibration gas. The recipe parameters include the mass numbers of the calibration gas components and can be modified in the recipe editor. The "GSC Matrix" editor specifies the concentration of each calibration gas component and its contribution on the related mass number. The gas specific calibration factors are required for the actual MCD measurement project. They are determined in the calibration project (GSC Result View) and saved in the MCD Calibration Factor Library.

Determining the GSC Factors

NOTE:

Before starting the measurement, check the correct calibration of the mass spectrometer components. If calibration is necessary, perform the following preparatory measurements:

- Calibrate the mass scale,
- Determine the offset.
- Determine the background.

NOTE:

Gas mixtures that contain components with overlapping masses are not suited for use as calibration gas. The same mass number must not be assigned to several components.

1. Feed a suitable calibration gas into the vacuum chamber.
2. Open the start page: In the **View** menu, click **Show Start Page**.
3. Click on the icon for the required device.
4. Create a new calibration project: In the "Templates" list, double-click e.g. **Gas Specific Calibration.qmt**. This way you create a new calibration project based on the selected template. You can modify it according to your needs.
5. The new measurement project window appears. The working area displays the calibration project.
 - Edit the recipe according to your needs (if necessary): Click the corresponding tab in the working area selection.
 - Display the measuring data: Click the corresponding tab in the working area selection.
6. Input the parameters which define the calibration gas in the "GSC Matrix" editor.
 - Use the commands of the related context menu to edit the measurement tasks and masses.
 - Note: Use an identical name for the gas component in an MCD project. Otherwise, QUADERA® cannot refer to this component. As an example, QUADERA® does not equate "O2" and "Oxygen".

NOTE:

You can start the measurement regardless whether the recipe editor or the working area has been selected.

7. Start the measurement: In the device status view, click on the "Start" icon. The connection to the device is automatically established. The device now receives the parameters for the current measurement task. The measurement is running automatically.

8. In the GSC Result View, check the measured values and the calculated calibration factors.

9. Click **Apply to MCD Calibration Factor Library** to save the calibration factors in the MCD calibration factor library. Note:

- New calibration factors are added to the MCD Calibration Factor Library,
- Current values replace existing data sets in the MCD Calibration Factor Library.

10. When required for future applications: save the calibration project as template (menu **File** > **Save as Template...**).

11. Close and save the measurement project. In the **File** menu, click **Close**. You are requested if you want to save the measurement project. QUADERA® suggests an automatically generated file name that is based on date/time of the measurement and the used template.

- Yes: the "Save As" window used for saving measuring data opens up. Select a suitable name and path and then click **Save**. The measurement project will be saved and closed. Please note: The file extension for measurement projects is *.qmp
- No (recommended option): the measurement project will be closed without saving the data.
- Cancel: the action is cancelled. You will return to the measurement project without saving the data.

GSC Matrix Editor

The parameters that define the calibration gas are displayed in the "GSC Matrix" editor of the calibration project. Each calibration gas component is defined by its name, concentration, and the measurement task(s). Use the "Add MCD Task" tool to add a new component (measurement task).

Image of "GSC Matrix" editor (example)

Parameter	Range	Description
<ul style="list-style-type: none"> Component 	Letters and digits	<p>Name of the calibration gas component.</p> <p>Note: In an MCD project, use an identical name for the gas component. Otherwise, QUADERA® cannot refer to this component. As an example, QUADERA® does not equate "O2" and "Oxygen".</p>
<ul style="list-style-type: none"> Concentration 	Number > 0	Concentration of the calibration gas component.
<ul style="list-style-type: none"> Mass 	(not editable)	<p>The gas specific calibration factors are determined for these measurement tasks: accepted from the MID recipe ("Task Name" parameter).</p>
<ul style="list-style-type: none"> Mass # 	Checkbox	<p>Defines whether a calibration factor for the component is determined in the corresponding measurement task, or not.</p> <p>Note:</p> <ul style="list-style-type: none"> Only one calibration factor can be calculated per measurement task. Several calibration factors per component can be determined at the same time. A red colored cell indicates the internal standard. Use the context menu of the "GSC Matrix" editor to set the internal standard.

Context menu of the "GSC Matrix" editor

In this context menu the following commands are available:

- **Delete selected Component:** delete the marked measurement task (table row) from the "GSC Matrix" editor.
- **Delete selected Mass:** delete the marked mass (table column) from the "GSC Matrix" editor.
- **Set as internal standard:** set the internal standard for the calibration factors.

Proceed as follows to set the internal standard for the calibration factors:

1. Open the context menu in the table element related to the mass/component pair you want to set as internal standard.
2. Click **Set as internal standard**. The table element for the internal standard appears with a red background color.

		Mass					
Component	Concentration	Mass 14	Mass 28	Mass 29	Mass 32	Mass 40	Mass 44
▶ Ar	0.93%	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
CO2	300ppm	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
N2	78.14%	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
O2	20.9%	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

GSC Result View

The parameters required to determine the calibration factors are displayed in the "GSC Result View" of the calibration project.

The "GSC Result View" displays the calibration factors in a tabular form. They are calculated for all measurement tasks of the MID recipe, using the corresponding measured data. In the course of time you can extend and complete the MCD Calibration Factor Library (function "Apply to MCD Calibration Factor Library") by using various calibration gases to determine the calibration factors.

Image of "GSC Result View" (example)

Parameter	Range	Description
<ul style="list-style-type: none"> Component 	(not editable)	Name of the calibration gas component: applied from the "GSC Matrix" editor ("Component" parameter).
<ul style="list-style-type: none"> Mass 	(not editable)	Measurement tasks for which the gas specific calibration factors are determined: applied from the related MID recipe ("Task Name" parameter).
<ul style="list-style-type: none"> Intensity 	(not editable)	Intensity at the related mass number: corresponds to the currently measured value for this mass number.
<ul style="list-style-type: none"> Factor 	(not editable)	The calibration factor is automatically calculated from the measured intensity and the specified concentration.
<ul style="list-style-type: none"> Apply to MCD Calibration Factor Library 	Button	Apply the current gas specific calibration factors to the MCD Calibration Factor Library. NOTE: <ul style="list-style-type: none"> New calibration factors are added to the MCD Calibration Factor Library, Current values replace existing data sets in the MCD Calibration Factor Library.

Component	Mass	Intensity	Factor
O2	Mass 32	8,124E-06	3,111E00
▶ N2	Mass 28	9,764E-06	1,000E00
Ar	Mass 40	1,630E-06	1,403E01
CO2	Mass 44	6,150E-08	1,641E01

MCD Calibration Factor Library

Measuring the concentration of the components of a gas mixture requires that the corresponding calibration factors are known. These are stored in the MCD Calibration Factor Library, in tabular form. Each calibration factor is defined in the related calibration project by the mass number and the name of the corresponding component.

The calibration factors are quantified relatively. This requires to set one calibration factor as the internal standard. Normally, the calibration factor for N₂ (m/e = 28) is used and set to 1 (standard setting). The other calibration factors relate to the standard. This approach allows you to create a consistent MCD Calibration Factor Library. Use the context menu of the "GSC Matrix" editor to set the internal standard.

Image of MCD Calibration Factor Library (example)

Extending the MCD Calibration Factor Library

Proceed as follows to extend the MCD calibration factor library:

1. Perform a new gas specific calibration (calibration project).
2. Apply the new calibration factors to the MCD Calibration Factor Library:
In the section of the calibration project, click **Apply to MCD Calibration Factor Library**.

Deleting the MCD Calibration Factor Library

1. Click **Delete MCD Calibration Factor Library** to remove all data sets from the MCD calibration factor library.

NOTE:

"Delete MCD Calibration Factor Library" deletes the data sets of the MCD Calibration Factor Library irretrievably. In this case, a new gas specific calibration is required for new data sets.

MCD Calibration Factor Library							
	14,00	16,00	18,00	28,00	32,00	40,00	44,00
Mass	14,00	16,00	18,00	28,00	32,00	40,00	44,00
Factor H2O	0,00	0,01	1,00	0,00	0,00	0,00	0,00
Factor Ar	0,00	0,00	0,00	0,00	0,00	1,00	0,00
Factor O2	0,00	0,10	0,00	0,00	0,87	0,00	0,00
Factor N2	0,10	0,00	0,00	1,00	0,00	0,00	0,00
Factor CO2	0,00	0,00	0,00	0,20	0,00	0,00	1,50

Enabling Partial Pressure

Determining the Sensitivity

The Device Sensitivity must be determined for the device to display Partial Pressure.

To determine the Sensitivity, run the Sensitivity Determination measurement project. Enter the Calibration Factors for each mass, enter the Total Pressure (if no gauge is attached) and run the measurement project.

The Device Sensitivity can then be saved to the software device.

Required Process to Enable Partial Pressure

To use Partial Pressure, the following must be done:

- An Offset Calibration must have been executed at some point. QUADERA will check to see if this has been done.
- A SEM Amplification Calibration must have been executed at some point. This determines the gain of the SEM.
- Calibration Factors must be set up using the Sensitivity Determination measurement project.
- The Sensitivity must be determined for the device using the Sensitivity Determination measurement project. A default Sensitivity is available but is not as accurate as a Sensitivity determined by QUADERA for the specific device.
- The Partial Pressure units must be selected (default is mbar).

Measurements using QUADERA

Measurement Projects and Measurement Project Templates

In QUADERA®, data are stored as measurement project templates and as measurement projects. Each measurement project template or measurement project is used for a specific measurement task.

Measurement project templates

Measurement project templates allow you to access frequently performed measurement tasks easily. Measurement project templates are created by INFICON or experienced users in order to keep the effort required for configuring typical measurement tasks at a minimum. Typical measurement project templates are installed together with QUADERA®. You can find these in the Start page.

In addition, QUADERA® provides basic templates for each measurement project, such as Scan, MID, MCD etc. These templates normally include just one measurement task and are intended to create user specific measurement project templates as starting points for future measurement projects.

Measurement projects

A measurement project contains the measuring data as well as an image of the device required for displaying the measuring data correctly.

	Measurement project template	Measurement project
File extension	*.QMT	*.QMP
Recipe definition	Yes	Yes
Configured sections	Yes, several	Yes, several
Device settings	Reference to the device type	Complete image of the device
Measuring data	No	Yes

Comparison: Measurement project template vs. measurement project

Scan Measurement Projects

In a scan-analog measurement, the ion current is measured as a function of m/e . This quickly allows you to make a qualitative statement such as "The gas consists of ..., ..., ..., of which ... represents the majority. The fraction of ... is very small or cannot be measured".

However, it is rather cumbersome to deduce the quantitative composition of the gas in % or ppm. Information about changes in the gas composition with time is hard to deduce from a sequence of several scans, and measurements over long periods of time also result in extremely large amounts of data.

In scan-analog measurement projects you can also add analog input tasks (e.g. via quadrupole controller QC, "EXT IN").

Scan-analog also allows for capturing and comparing a reference scan if using a reference-based measurement project.

A separate measurement project - Bargraph Cycles - can be used to plot analog scans against time.

QUADERA® also provides a scan-analog measurement project template that displays a 3D graph of analog scans. 3D consumes system resources and should be used for only short periods of time, if possible.

NOTE:

A precise measurement requires the correct calibration of the components of the mass spectrometer.

See Example for the course of a scan measurement project (measure_example_scan).

NOTE:

For a written documentation of your measurement projects you can capture screens of the QUADERA® user interface. Reports can also be printed from a selection on the context menu.

MID Measurement Projects

In an MID measurement (Multiple Ion Detection) you specify distinct m/e values for which the ion current is to be measured. Only the specified mass numbers are scanned in this case. Each of these mass numbers is represented by a separate measurement task for which all parameters can be set.

Changes in the gas composition with time can be recorded and displayed easily. An additional analysis of the measuring data allows you to convert the results into concentrations given in %, ppm, etc (MCD measurement).

MID Measurement data can be displayed in amps or partial pressure. To display in partial pressure, one must first run the offset calibration measurement, calibrate the SEM Amplification, then determine the device sensitivity and lastly set the partial pressure units.

- The Sensitivity of the instrument is the ratio of the ion current measured for a given mass to the partial pressure of a gas.
- Only one Sensitivity parameter exists in QUADERA. It is used to calculate Partial Pressures for measurements using the Faraday or SEM detector.
- Partial Pressure also uses a Calibration Factor, which is the ratio of the total ion current (at all masses) produced from a given partial pressure of that substance, to the total ion current produced from nitrogen at the same partial pressure. The Calibration Factor(s) depends strongly on the energy of the ionizing electrons. If the correct values of the Calibration Factors are not known for the exact conditions of the particular analyzer being used, they can be approximated using published relative ion gauge sensitivities for various gases.
- If the SEM voltage is changed after SEM Amplification and Sensitivity have been determined then Partial Pressure calculations will be less accurate. If changing the SEM voltage, it is best to calibrate the SEM Amplification and determine the Sensitivity again before using Partial Pressure.

NOTE: Setting or changing the partial pressure units requires one full scan through the MID measurement tasks to correctly update the chart.

NOTE:

A precise measurement requires the correct calibration of the components of the mass spectrometer.

See Example for the course of an MID measurement project (measure_example_sample).

NOTE:

For a written documentation of your measurement projects you can capture screens of the QUADERA® user interface. Reports can also be printed from a selection on the context menu.

MCD Measurement Projects

The MCD measurement (Multiple Concentration Determination) is based on an MID measurement project and includes additional evaluation to measure concentrations. A matrix of calibration factors (analysis matrix) is used to convert the measured ion currents into concentrations of the individual gas components. The calibration factors are not universally valid. They must be quantified by a separate measurement using calibration gases, i.e. one or more GSC measurements. The actual MCD measurement and the calibration are closely connected.

NOTE:

A precise measurement requires the correct calibration of the mass spectrometer components.

1. Before starting the measurement, check the correct calibration of the components of the mass spectrometer. If calibration is necessary, perform the following preparatory measurements:
 - Calibrate the mass scale,
 - Measure the offset,
 - Determine the background of the mass spectrometer,
 - Quantify the gas specific calibration factors.
2. Open the start page: In the **View** menu, click **Show Start Page**.
3. Click on the icon for the required device.
4. Create a new MCD measurement project: In the "Templates" list, double-click the desired measurement project template. This way you create a new measurement project based on the selected template.
 5. The new measurement project window appears. The working area displays the MCD project.
 - Edit the MCD recipe if necessary: click the corresponding tab in the working area selection,
 - Display the measuring data: click the corresponding tab in the working area selection.

NOTE:

You can start the measurement regardless whether the recipe editor or the working area has been selected.

6. Start the measurement: In the device status view, click on the "Start" icon. The connection to the device is automatically established. The device now receives the parameters for the current measurement task. You can adjust the chart layout while the measurement is running.
 7. Stop the measurement: In the device status view, click on the "Stop" icon.

8. Close and save the measurement project. In the **File** menu, click **Close**. You are requested if you want to save the measurement project. QUADERA® suggests an automatically generated file name that is based on date/time of the measurement and the used template.
- Yes: the "Save As" window used for saving measuring data opens up. Select a suitable name and path and then click **Save**. The measurement project will be saved and closed.
Please note: The file extension for measurement projects is *.qmp
 - No: the measurement project will be closed without saving the data.
 - Cancel: the action is cancelled. You will return to the measurement project without saving the data.

NOTE:

For a written documentation of your measurement projects you can capture screens of the QUADERA® user interface. Reports can also be printed from a selection on the context menu.

Total Pressure Measurement

This chapter is valid for the QMG220 only.

QUADERA® supports total pressure measurements in the vacuum system (hardware supported only for QMG220). This requires that an appropriate pressure gauge is connected to the QMG and the device settings are adjusted accordingly. The total pressure measurement is available for:

- Scan measurement projects,
- MID measurement projects,
- MCD measurement projects.

Use the recipe editor to add the measurement task "Total Pressure" to the measurement project. The measured data (total pressure in the vacuum system) are displayed and saved. Besides, the course of a measurement corresponds to the selected measurement project.

Adding the measurement task "Total Pressure" to a recipe

Apply the "Add Total Pressure Task" or "Add Total Pressure Task to Chart" tools to the recipe editor. Edit the recipe parameters if necessary.

Further notes

Pay attention to the following items when measuring the total pressure:

- The pressure gauge is not permanently switched on because the plasma in the gauge influences the gas composition in the recipient. Exception: monitoring the QMG.
- Note that igniting the pressure gauge and displaying the correct pressure will take some time (refer to the operating instructions for the pressure gauge).

NOTE:

For a written documentation of your measurement projects you can capture screens of the QUADERA® user interface. Reports can also be printed from a selection on the context menu.

Creating Measurement Project Templates

Proceed as follows to create a new measurement project template:

1. Use e.g. the start page to open an existing measurement project template, or an existing measurement project.
2. Use the recipe editor to modify the recipe parameters according to your needs.
3. Use the toolbox to change the working area according to your needs.
4. In the **File** menu, click **Save As Template....** Select the path for the measurement project template, and input the file name.

Note:

- By default, the path set in the options is used for new measurement project template,
- The file extension *.qmt is used for measurement project templates.

Recipes

Recipes

A recipe contains a sequence of measurement tasks. Use the recipe editor to change the recipe parameters.

The following recipe types are available:

- Scan recipes: parameters for *scan-analog measurement project*

In a scan-analog measurement, the ion current is measured as a function of m/e. This quickly allows you to make a qualitative statement such as "The gas consists of ..., ..., ..., of which ... represents the majority. The fraction of ... is very small or cannot be measured".

However, it is rather cumbersome to deduce the quantitative composition of the gas in % or ppm. Information about changes in the gas composition with time is hard to deduce from a sequence of several scans, and measurements over long periods of time also result in extremely large amounts of data.

In scan-analog measurement projects you can also add total pressure measurement tasks (for the QMG220, if a pressure gauge is installed) and analog input tasks (AI).

- MID recipes: parameters for *MID/MCD measurement project*

In an MID measurement (Multiple Ion Detection) you specify distinct m/e values for which the ion current is to be measured. Only the specified mass numbers are scanned in this case. Each of these mass numbers is represented by a separate measurement task for which all parameters can be set.

Changes in the gas composition with time can be recorded and displayed easily. An additional analysis of the measuring data allows you to convert the results into concentrations given in %, ppm, etc. (MCD measurement).

In MID measurement projects you can also add total pressure measurement tasks (for the QMG220, if a pressure gauge is installed) and analog input tasks (AI).

- MCD recipes: additional parameters for *MCD measurement project*

The MCD measurement (Multiple Concentration Determination) is based on a MID measurement project and includes additional evaluation to measure concentrations. A matrix of calibration factors (analysis matrix) is used to convert the measured ion currents into the concentrations of the individual gas components. The calibration factors are not universally valid. They have to be quantified by a separate measurement using calibration gases.

In MCD measurement projects you can also add total pressure

measurement tasks (for the QMG220, if a pressure gauge is installed) and analog input tasks (AI).

NOTE:

New or modified parameters for the measurement tasks are accepted by the device only after the measurement has been restarted.

Recipe Editor

In the working area selection, click the corresponding tab. The recipe parameters for the active recipe are displayed in the section in tabular form (recipe editor). The columns represent the measurement tasks and the rows represent the recipe parameters.

Editing parameters

Proceed as follows to edit a parameter:

1. Click the required cell.
2. Depending on the parameter type:
 - Enter the required parameter via the keyboard, or
 - Use the spin buttons to modify the parameter, or
 - Select the required parameter in the respective dropdown list.
3. After a parameter has been input, an automatic check is normally performed to ensure that the parameter lies within the permitted range. This prevents bad data input, and facilitates correct input.
4. The parameter is accepted automatically as soon as you leave the cell.

Add measurement task

Proceed as follows to add a new measurement task to the recipe:

1. Use the tool that is applicable to the measurement project:
 - "Add Scan Task" for scan measurement projects.
 - "Add Peak Task" for scan measurement projects.
 - "Add MID Task" for MID and MCD measurement projects.
 - "Add MCD Task" for MCD measurement projects.
 - "Add Total Pressure Task" for Scan, MID and MCD measurement projects,
 - "Add Analog Input Task" for Scan, MID and MCD measurement projects.

Change sequence of measurement tasks

Proceed as follows to change the sequence of measurement tasks in a recipe:

1. Select the column that corresponds to the measurement task.
2. Drag&Drop the measurement task to the required position. A red arrow indicates the insert position.

Delete measurement task

Proceed as follows to delete a measurement task from the recipe:

1. Select the entire column that corresponds to the measurement task.
2. On the keyboard, click the **Del** key (delete), or use the context menu. When the measurement task contains data a requester appears and queries you to approve deleting.

Context menu of the recipe editor

This context menu contains the following functions

- **Copy Parameter To All:** applies the selected parameter to all measurement tasks.
- **Delete selected Task:** deletes the selected measurement task.

NOTE:

New or modified parameters for the measurement tasks are accepted by the device only after the measurement has been restarted.

Recipe Parameters: Scan

NOTE:

New or modified parameters for the measurement tasks are accepted by the device only after the measurement has been restarted.

The following recipe parameters are available:

Task Name

First Mass

Width

Speed

Dwell

Mass Mode

Detector Type

AI Channel

Gain (only QMG700)

SEM Voltage

CP-Level (only QMG700)

Autorange Mode

Detector Range

Range Limit

Analog Signal Filter (only QMG700)

Resolution

Pause Calibrate

AO Channel

AO Mode (only QMG220)

AO Range (only QMG220)

Trip Type

Level A

DO# A

Level B

DO# B

State

Parameter	Range	Description
-----------	-------	-------------

QUADERA HTML Help

- **Task Name** Letters and digits Name of the measurement task.
Note that for analog input scan measurement tasks the trip function and the related parameters are available.
- **First Mass** Number > 0 Start mass for the measurement.
Enter the required value or use the spin buttons.
- **Width** Any number Mass range to be scanned (starting with the start mass).
Reverse scans, i.e. from right to left, are performed for negative values.
Enter the required value or use the spin buttons.
- **Speed** Dropdown list Measuring time per mass for scan measurements (mass scan)
- **Dwell** Dropdown list Dwell time for the measurement of the analog input of the QC (only relevant for detector type EXT_IN_# in analog input measurement tasks).
- **MassMode** Dropdown list Operation mode for scan-analog measurements and peak tasks:
 - SCAN-N (only scan-analog measurements):
Ion currents are detected in a mass scan.
 - SCAN-F (only scan-analog measurements):
Ion currents are additionally filtered using a FIR algorithm (FIR: Finite Impulse Response). The filter removes in large part interfering noise from the raw signal of the electrometer preamplifier. Thus, even very small peaks can be detected in the background signal.
 - STAIR-T (only peak tasks):
Record a mass spectrum with integer mass jumps.
 - PEAK-L (only peak tasks):
Scan-analog measurement with threshold value. Only that

		peaks are recorded and displayed, which exceed the threshold value.
		<ul style="list-style-type: none"> • PEAK-F (only peak tasks): Ion currents are additionally filtered using a FIR algorithm.
• Detector Type	Dropdown list	Used detector type.
• AI Channel	Dropdown list	Number of the analog input for measuring data (only relevant for detector type AI in analog input measurement tasks).
• Gain	Dropdown list	Parameter valid only for QMG700 Measuring range for the analog input of the QC (only relevant for detector type EXT_IN_# in analog input measurement tasks).
• SEM Voltage	Number > 0	Operating voltage for the SEM. Enter the required value or use the spin buttons. The value "0" means that the common SEM voltage is applied. It is displayed and set in the device status view.
• CP-Level	Number > 0	Parameter valid only for QMG700 Response threshold of the ion counter preamplifier.
• Autorange Mode	Dropdown list	In QUADERA®, the amplifier measuring range can be fixed or adjusted automatically. <ul style="list-style-type: none"> • FIX: You can select the measuring range under Amplifier Range. • AUTO: The measuring range is selected automatically from all possible ranges. • AUTO-DOWN: The measuring range is selected automatically from all ranges located between the largest (least sensitive) range and the Range Limit.
• Detector	Dropdown list	Measuring range for the ion

	Range		current (only relevant for Autorange Mode=FIX)
•	Range Limit	Dropdown list	Most sensitive measuring range for the ion current (only relevant for Autorange Mode=AUTO-DOWN)
•	Analog Signal Filter	Dropdown list	Parameter valid only for QMG700 Time constant of analog filter.
•	Resolution	Integer number > 0	Mass resolution (small number = clear separation of peaks). Typical values are approx. 25 for QMG700, and approx. 50 for QMG220. Enter the required value or use the spin buttons.
•	Pause Calibrate	Number > 0	A factor used to multiply the pause time determined in the device. In order to wait for transient effects, no measurements are performed during the pause time between two measurement tasks. Enter the required value or use the spin buttons.
•	AO Channel	Dropdown list	Number of the analog output. Measured values are output to this AO.
•	AO Mode	Dropdown list	Parameter valid only for QMG220 Scales the measurement signal output (0&ldots;10 V). Parameter valid only for specified AO Channel.
•	AO Range	Dropdown list	Parameter valid only for QMG220 Adjusts the measurement range to the maximum measured signal output. Parameter valid only for specified AO Channel.
•	Trip Type	Dropdown list	Parameter valid only for analog input and total pressure measurement tasks. The trip function can monitor measurement values of analog input measurements. Each measurement task provides two trip functions, A and B, and the related threshold values, Level A and Level B. The trip function

results are sent to the output Bits DO# A and DO# B.

- OFF:
The trip function is switched off.
 - ABS:
Use the trip function "ABS" for vacuum monitoring, differential pressure monitoring, and as comparator. Read further information.
 - HYST:
Use the trip function "HYST" to prevent permanent switching for fluttering signals. Read further information.

- Level A Number Threshold value A (available only for trip types ABS and HYST).

- DO# A Integer number > 0 Digital output Bit. The result of the trip function is output to this DO (available only for trip types ABS and HYST).

- Level B Number Threshold value B (available only for trip types ABS and HYST).

- DO# B Integer number > 0 Digital output Bit. The result of the trip function is output to this DO (available only for trip type ABS).

- State Dropdown list Status of the measurement task.
 - ENABLE:
The measurement task is being measured and the parameters are being saved.
 - SKIP:
The measurement task is not being measured, but the parameters are preserved.

Recipe Parameters: MID

NOTE:

New or modified parameters for the measurement tasks are accepted by the device only after the measurement has been restarted.

The following recipe parameters are available:

Task Name

Mass

Dwell

Detector Type

AI Channel

Gain (only QMG700)

SEM Voltage

CP-Level (only QMG700)

Autorange Mode

Detector Range

Range Limit

Analog Signal Filter (only QMG700)

Resolution

Pause Calibrate

AO Channel

AO Mode (only QMG220)

AO Range (only QMG220)

Trip Type

Level A

DO# A

Level B

DO# B

State

Parameter	Range	Description
• Task Name	Letters and digits	Name of the measurement task
• Mass	Number > 0	Mass number for the measurement task.

		Enter the required value or use the spin buttons.
• Dwell	Dropdown list	Dwell time for the measurement at the current mass. In analog input measurement tasks: Dwell time for the measurement of the analog input of the QC (only relevant for detector type EXT_IN_#).
• Detector Type	Dropdown list	Used detector type
• AI Channel	Dropdown list	Number of the analog input for measuring data (only relevant for detector type AI in analog input measurement tasks).
• Gain	Dropdown list	Parameter valid only for QMG700 Measuring range for the analog input of the quadrupole controller QC (only relevant for detector type EXT_IN_# in analog input measurement tasks).
• SEM Voltage	Number > 0	Operating voltage for the SEM. Enter the required value or use the spin buttons. The value "0" means that the common SEM voltage is applied. It is displayed and set in the device status view.
• CP-Level	Number > 0	Parameter valid only for QMG700 Response threshold of the ion counter preamplifier.
• Autorange Mode	Dropdown list	In QUADERA®, the amplifier measuring range can be fixed or adjusted automatically. <ul style="list-style-type: none"> • FIX: You can select the measuring range under Amplifier Range. • AUTO: The measuring range is selected automatically from all possible ranges. • AUTO-DOWN: The measuring range is

selected automatically from all ranges located between the largest (least sensitive) range and the Range Limit.

- Detector Range Dropdown list Measuring range for the ion current (only relevant for Autorange Mode=FIX)
- Range Limit Dropdown list Most sensitive measuring range for the ion current (only relevant for Autorange Mode=AUTO-DOWN)
- Analog Signal Filter Dropdown list Parameter valid only for QMG700
Time constant of analog filter.
- Resolution Integer number > 0 Mass resolution (small number = clear separation of peaks). Typical values are approx. 25 for QMG700, and approx. 50 for QMG220.

Enter the required value or use the spin buttons.
- Pause Calibrate Number > 0 A factor used to multiply the pause time determined in the device. In order to wait for transient effects, no measurements are performed during the pause time between two measurement tasks.

Enter the required value or use the spin buttons.
- AO Channel Dropdown list Number of the analog output. Measured values are output to this AO.
- AO Mode Dropdown list Parameter valid only for QMG220

Scales the measurement signal output (0...10 V). Parameter valid only for specified AO Channel.
- AO Range Dropdown list Parameter valid only for QMG220

Adjusts the measurement range to the maximum measured signal output. Parameter valid only for specified AO Channel.
- Trip Type Dropdown list The trip function can monitor measurement values of MID- and MCD measurements, total pressure measurements, and analog input measurements (AI). Each measurement task provides

two trip functions, A and B, and the related threshold values, Level A and Level B. The trip function results are sent to the output Bits DO# A and DO# B.

- OFF:
The trip function is switched off.
 - ABS:
Use the trip function "ABS" for vacuum monitoring, differential pressure monitoring, and as comparator. Read further information.
 - HYST:
Use the trip function "HYST" to prevent permanent switching for fluttering signals. Read further information.
- | | | |
|-----------|--------------------|--|
| • Level A | Number | Threshold value A (available only for trip types ABS and HYST). |
| • DO# A | Integer number > 0 | Digital output Bit. The result of the trip function is output to this DO (available only for trip types ABS and HYST). |
| • Level B | Number | Threshold value B (available only for trip types ABS and HYST). |
| • DO# B | Integer number > 0 | Digital output Bit. The result of the trip function is output to this DO (available only for trip type ABS). |
| • State | Dropdown list | <p>Status of the measurement task.</p> <ul style="list-style-type: none"> • ENABLE:
The measurement task is being measured and the parameters are being saved. • SKIP:
The measurement task is not being measured, but the parameters are preserved. |

Recipe Parameters: MCD

NOTE:

New or modified parameters for the measurement tasks are accepted by the device only after the measurement has been restarted.

An MCD measurement project is based on an MID measurement project and includes additional evaluation to yield the components' concentrations of a gas mixture (quantitative gas analysis). Thus, an MCD measurement project always contains a measurement recipe and an analysis matrix which contains the gas specific calibration factors. The MCD measurement project is closely related to a gas specific calibration which is needed to determine the relevant calibration factors. Note that you should perform the gas specific calibration directly before the MCD measurement project.

Analysis matrix (MCD Matrix Editor)

The analysis matrix connects the MID measurement recipe with the gas components:

- The rows of the analysis matrix are defined by the name of the gas components for the quantitative analysis.
- Use the "Add MCD Task" tool to add a row (gas component) to the matrix.

NOTE:

In the MCD project, use identical names for the gas components as used in the gas specific calibration. Otherwise, QUADERA® cannot refer to the components. As an example, QUADERA® does not equate "O2" and "Oxygen".

- The columns of the analysis matrix are defined by the measurement recipe, and correspond to the mass numbers in the measurement tasks.
- The individual matrix elements represent the gas specific calibration factors for the quantitative gas analysis. The calibration factors are determined in the gas specific calibration and stored in the MCD Calibration Factor Library.

Recipe Parameters: Total Pressure

This chapter is valid for the QMG220 only.

NOTE:

New or modified parameters for the measurement tasks are accepted by the device only after the measurement has been restarted.

The following recipe parameters are available: :

Task Name

Dwell

Detector Type

Trip Type

Level A

DO# A

Level B

DO# B

State

Parameter	Range	Description
• Task Name	Letters and digits	Name of the measurement task.
• Dwell	Dropdown list	Dwell time for the measurement of the total pressure.
• Detector Type	(not editable)	Detector type "TotalPressure": installed total pressure gauge
• Trip Type	Dropdown list	<p>The trip function can monitor measurement values of total pressure measurements. Each measurement task provides two trip functions, A and B, and the related threshold values, Level A and Level B. The trip function results are sent to the output Bits DO# A and DO# B.</p> <ul style="list-style-type: none"> • OFF: The trip function is switched off. • ABS: Use the trip function "ABS" for vacuum monitoring, differential

- pressure monitoring, and as comparator. Read further information.
 - HYST:
Use the trip function "HYST" to prevent permanent switching for fluttering signals. Read further information.
- Level A Number Threshold value A (available only for trip types ABS and HYST).
- DO# A Integer number > 0 Digital output Bit. The result of the trip function is output to this DO (available only for trip types ABS and HYST).
- Level B Number Threshold value B (available only for trip types ABS and HYST).
- DO# B Integer number > 0 Digital output Bit. The result of the trip function is output to this DO (available only for trip type ABS).
- State Dropdown list Status of the measurement task.
 - ENABLE:
The measurement task is being measured and the parameters are being saved.
 - SKIP:
The measurement task is not being measured, but the parameters are preserved.

Trip Function ABS

Use the trip function "ABS" for the following purposes:

- Vacuum monitoring,
- Differential pressure monitoring,
- Windows comparator.

Vacuum monitoring

Requires just the trip function Trip A. Proceed as follows to use the trip function for vacuum monitoring in MID and MCD measurement projects:

1. Select trip type "ABS".
2. Enter the threshold value "Level A".
3. Set the digital output Bit "DO# A". The result of the trip function is output to DO# A.

The trip function ABS-Trip A switches on when the signal falls below Level A.



Differential pressure monitoring

Requires just the trip function Trip B. Proceed as follows to use the trip function for differential pressure monitoring in MID and MCD measurement projects:

1. Select trip type "ABS".
2. Enter the threshold value "Level B".
3. Set the digital output Bit "DO# B". The result of the trip function is output to DO# B.

The trip function ABS-Trip B switches on when the signal exceeds Level B.




Windows Comparator

Requires the two trip function Trip A and Trip B. Proceed as follows to use the trip functions as comparator in MID and MCD measurement projects:

1. Select trip type "ABS".
2. Enter the upper threshold value "Level A".
3. Enter the lower threshold value "Level B".
4. Set identical values to the digital output Bits "DO# A" and "DO# B", i.e. DO# A:xx and DO# B:xx. The two trip functions are conjoined (logical operator AND).

The trip function ABS switches on when the signal is in the range between the threshold values Level B and Level A.

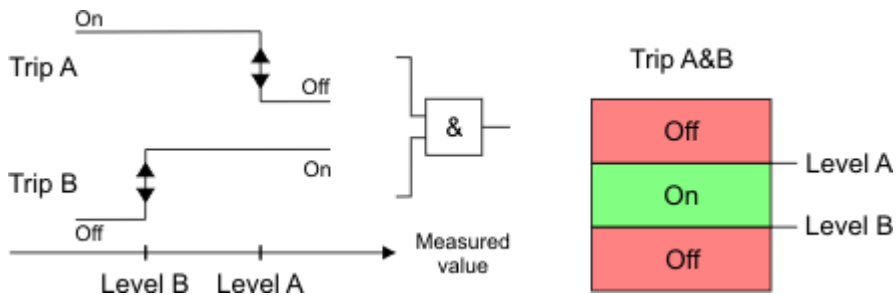


Trip Function HYST

Use the trip function "HYST" (hysteresis) to prevent permanent switching for fluttering signals.

This requires just the trip function Trip A. Proceed as follows to use the hysteresis trip function "HYST" in MID and MCD measurement projects:

1. Select trip type "HYST".
2. Enter the lower threshold value "Level A".
3. Enter the upper threshold value "Level B".
4. Set the digital output Bit "DO# A". The result of the trip function is output to DO# A.

The trip function HYST switches on when the signal falls below Level A, and it switches off when the signal exceeds Level B.

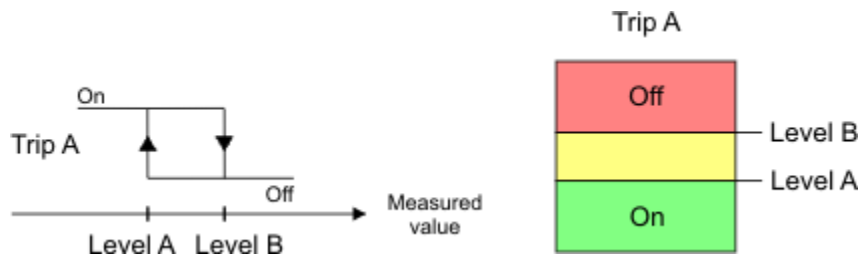

Processing Measurement Data

Minimum

Action

Return the smallest measuring value found in the selected part of the measuring curve:

Minimum = Minimum(x_1, x_2, \dots, x_n),

$x_1 \dots x_n$ = Measuring values 1 ... n in the selected part

The calculation is updated continuously while the measurement is running.

Average

Action

Calculate the average value for all measuring values located in the selected part of the measuring curve:

$$\text{Average} = \frac{\sum x_i}{n},$$

x_i = Measuring value; n = number of measuring values in the selected part

The calculation is updated continuously while the measurement is running.

Maximum

Action

Return the largest measuring value found in the selected part of the measuring curve:

Maximum = Maximum(x_1, x_2, \dots, x_n),
 $x_1 \dots x_n$ = Measuring values 1 ... n in the selected part

The calculation is updated continuously while the measurement is running.

Absolute Standard Deviation

Action

Calculate the absolute standard deviation for all measuring values located in the selected part of the measuring curve:

$$\text{STDABS} = \sqrt{\frac{\sum x_i^2 - n \cdot \text{Average}^2}{n-1}},$$

x_i = Measuring value; n = number of measuring values in the selected part

The calculation is updated continuously while the measurement is running.

Automating Tasks

Triggered Run Add-in

The purpose of the Triggered Run Add-in (installed with QUADERA 4.40) is to provide a QUADERA Add-in that automates the execution of multiple QUADERA operations. These operations include loading a Template, running the associated Measurement Project, saving its data, and then exporting that data into an ASCII file. These operations are combined into what is referred to as a Triggered Run Task. The Add-in has the ability to create and configure a list of these tasks prior to run time. The Add-in also manages configuration of the execution of this task list by means of digital input triggering.

The Add-in provides the following functionality:

- Allows multiple Triggered Run Tasks, where each task can be configured so that:
 - A Template can be selected.
 - The Save Files can be defined. (Save file is of type .qmp, and the exported ASCII file will have the same name, with the .asc extension.)
 - The Filament can be turned on or off.
 - The SEM can be turned on or off.
- Allows the user to select the desired QMG device.
- Allows the user to select the Digital Input to be used as the Trigger.
- Allows the user to select the how the Digital Input should be used:
 - The QMG can run when the Digital Input switches on and then stop when it switches off.
 - The QMG can run when the Digital Input switches off and then stop when it switches on.
- Allows automatic preparation of the system, so that all Measurement Files have been opened and the QMG is ready to run.
- Allows the user to begin watching for triggers.
- Allows the user to stop watching for triggers.
- Requires user approval prior to exporting data.
- Automatically manages switching through the list of Tasks.
- Allows the user to save all configuration information.

This sequence of steps should be followed to run the Triggered Run Add-in:

- Select QMG – In the list labeled “Select QMG” choose the QMG to be used for the run. Only one QMG can be selected for a run.

- Configure the Task List – A Task is an operation that uses a given template to open a Measurement File, configures the QMG Filament and SEM, runs that QMG and then finally saves and exports the associated data.
 - Add New – Using the text boxes under the list view, define the parameters of a new Task.
 - Template – Enter the name of an existing template stored in the default template directory, including .qmt extension, or use the browse button to navigate to the desired template.
 - Save As – Enter in the name to give the saved Measurement File, including extension .qmp. This entered File name will also be used to save the exported ASCII file, but it will use the .asc extension instead.
 - Filament – Check “Filament” if it is desired for this task to be run with the filament turned on.
 - SEM – Check “SEM” if it is desired to run this task with the SEM turned on.
 - Click “Add Task” and a new row will be added to the table with the parameters as defined above.
 - Update Task – When a task is selected in the table, the fields for editing are automatically filled. The user can modify any or all of the fields and then click the “Update Task” button. The selected row will be updated with the new values.
 - Delete Task – When one or more rows are selected in the table, and the “Delete task” button is clicked, those rows will be removed.
 - No changes are saved until the “Save” button is clicked or “Ok” is used to dismiss the dialog.
- Configure the Run – The Run (i.e. how all tasks will be executed) can be configured by the controls in the group labeled “Manage Running of Tasks”.
 - Connect – Connect executes the task of making a connection between QUADERA and the QMG device. You must connect prior to configuring the Run. Certain information is only available after connection. If the Button says “Connect” then you must connect to the selected QMG. If the button says “Disconnect” then the QMG is already connected and you are ready to configure.
 - “Run while DI On” indicates that the user wants each task to start and run when the Digital Input indicated changes state to “On” (if checked) or “Off” (if not checked).
 - If “Run while DI On” is checked, then when the Digital Input changes to “On”, the next task will begin running. When that Digital Input changes to “Off”, it will stop the task from running.
 - If “Run while DI On” is not checked, then when the Digital Input changes to “Off”, the next task will begin running. When that Digital Input changes to “On”, it will stop the task from running.

- “Run while DI On” is used for immediately starting the run if the start condition is true. After clicking the “Start” button, the run will begin with out waiting for a change in the Digital Input.
- “Digital Input to watch” is a list ranging from 1 to the number of Digital Inputs in the QMG device. This indicates which Digital Input will be used as the trigger for the run.
- “Reload when Finished” indicates that the scheduled run will be reloaded after completing the previous run. The next run is loaded, but it will not start watching for triggers until the “Start” button has been clicked. The next set of files will have their name appended with an index “(#)”. This will increment and the runs will continue reloading until the Add-in has been dismissed.
- “Restart after Reload” will be enabled if “Reload when Finished” has been checked. Using “Restart after Reload” skips the need for the user to click on “Start” after each run. The Add-in will immediately begin watching for triggers as soon as it has completed reloading.
- “Start” – Click “Start” after both the tasks and the Run have been configured. This will tell the Add-in to begin loading Measurement Files and to prepare for the Run. The Add-in will begin watching for value changes on the selected Digital Input. When that Digital Input changes value it triggers the Add-in to take action by either starting or stopping the current Task. By using these Triggers, the Add-in starts and stops each Task, iterating through the list until they have all been executed.
- “Stop” – Once the “Start” button has been clicked, the button text will change to “Stop”. Clicking the button at this point will manually stop the run.
- Completion of the run – When the run has been completed, the Add-in will automatically save the data file and export the data.

Scripting

Scripting

Scripting has been integrated into the host application, enabling the user to adapt the functions of the application to his or her needs. Scripting always requires the host application in order to be executed.

The Visual Studio Tools for Applications (VSTA) development system is suited to customize applications by using the .NET framework. VSTA replaces Visual Basic for Applications (VBA) and uses Visual Studio as the IDE.

With scripting, you can develop your own solutions to problems and in this way automate and extend the functions of the application. You can develop solutions that extend the functions of your application and that may be used again and again. By integrating VSTA, QUADERA® provides the user with a widely used and supported programming environment.

Scripting within QUADERA®

QUADERA® stores scripting code in a main scripting directory. The individual modules (add-ins) are stored separately. When required, the add-ins are available for all measurement project templates.

QUADERA® provides examples for add-ins and measurement project templates that use these Add-ins. You can use the templates via the start page.

NOTE:

For further information on scripting and the programming environment, please refer to the help file for Microsoft Visual Studio Tools for Applications. Use the Help menu of the VSTA editor.

NOTE:

The help system for the scripting functions within QUADERA® explains the extended instruction set and the corresponding syntax.

NOTE:

The QUADERA® Release Notes ("Readme.html" file) provide a description of "Saving VBA code for reprogramming in VSTA" to support users who have been working with VBA up to now.

Scripting Directory Structure

File types

A scripting add-in contains the following file types:

- Add-in DLL:
.Net assembly which contains the compiled add-in code (*.dll),
- Source code:
These are the files which allow the user to view, edit and compile the add-in. The main file is a "Visual Basic .Net" project (*.vbproj) which then contains links to other files such as VB.Net code (*.vb).

Directories

Scripting add-ins are stored by default in the directory "My Documents\My Quadera\Scripting":

- The sub-directory "MeasureProjectAddIns" contains the add-in DLL Files,
- The sub-directory "Code" contains the source code files. Each add-in is stored in a separate directory.

Add-ins which are present in the "MeasureProjectAddIns" directory can be used by QUADERA and will be listed in the "Add-in Manager" dialog. An add-in does not need to have source code available. However, without this the user will be unable to view or edit the code.

Example

The following table shows an example file structure for an add-in with the name "Sample":

(directories appear in normal type, files in italics)

📁 Scripting	
📁 MeasureProjectAddIns	◆ <i>Sample.dll</i>
📁 Code	
📁 Sample	◆ <i>Sample.vbproj</i>
	◆ <i>ThisMeasureProject.vb</i>
	◆ <i><Other source code files></i>

Note that you can change the file location of the scripting directory.

Copying Add-ins

Proceed as follows to copy an add-in:

1. Copy the add-in DLL file to the "MeasureProjectAddIns" directory.
2. If source code is also available:
 - a. Create a new directory under "Code" with the name of the add-in (without the DLL extension!).
 - b. Copy the source code files to this directory.

Deleting Add-ins

NOTE:

Add-ins can be used by more than one measurement project. Care should be taken when deleting an add-in.

Proceed as follows to delete an add-in:

1. Remove the add-in DLL file from the "MeasureProjectAddIns" directory.
2. If source code is also available: Remove the directory with the add-in name from the "Code" directory.

Using Macros

Creating Add-ins and Macros

In VSTA, an add-in can include more than one function. Each function can be considered as a macro and an add-in as "macro collection". Thus, you have two options to create a new macro:

- Edit an existing add-in to include a new function that can be used as macro,
- Create a new add-in and program a function that can be used as macro.

The following steps describe how to create a new add-in.

1. Open an existing measurement project, or create a new measurement project.
2. In the **Tools** menu, point to **Programming**.
3. In the submenu, select **Create Add-in....** The "Create Add-in" window opens up.
4. Use the field to specify the name of the add-in.
5. Click **[OK]**. The VSTA editor opens up. Now you can create the new add-in:
 - VSTA automatically creates the basic structure of the add-in that is executable without any functions,
 - Then you can program your own functions to expand the add-in.

QUADERA® stores each add-in in a main scripting directory. When required the add-ins are available for all measurement project templates.

NOTE:

For further information on scripting and the programming environment, please refer to the help file for Microsoft Visual Studio Tools for Applications. Use the Help menu of the VSTA editor.

Activating Add-ins

1. Open an existing measurement project, or create a new measurement project.
2. In the **Tools** menu, point to **Programming**.
3. In the submenu, select **Add-in Manager....** The "Add-in Manager" window opens up.
4. In the displayed "Available Add-ins" list, enable the checkbox next to the name of the required add-in.
5. Click **[OK]**.

Running Macros

Automatic run

QUADERA® automatically executes macros in the following cases:

- An add-in is loaded and its startup code calls up the macro,
- A QUADERA® event calls up the macro.

Manual run

You have to activate the relevant add-in before you can manually execute the macro.

1. In the **Tools** menu, point to **Programming**.
2. In the submenu, select **Macros...** The "Macros" window opens up.
3. In the displayed macro list, click the name of the macro to be executed (not the checkbox).
4. Click **Run**.

NOTE:

You can call up the "Macros" window with the keyboard shortcut ALT+F8.

Editing Add-ins and Macros

In VSTA, an add-in can include more than one function. Each function can be considered as a macro and an add-in as "macro collection". Proceed as follows to edit an add-in or an included macro:

1. Open an existing measurement project, or create a new measurement project.
2. In the **Tools** menu, point to **Programming**.
3. In the submenu, select **Add-in Manager....** The "Add-in Manager" window opens up.
4. In the displayed "Available Add-ins" list, click the name of the add-in to be edited, or browse for the required add-in.
5. Click **[Edit]**. The source code will then be opened in the VSTA editor for editing.

QUADERA® stores each add-in in a main scripting directory. When required, the add-ins are available for all measurement project templates.

NOTE:

For further information on scripting and the programming environment, please refer to the help file for Microsoft Visual Studio Tools for Applications. Use the Help menu of the VSTA editor.

Calling Up the VSTA Editor

1. Open an existing measurement project, or create a new measurement project.
2. In the **Tools** menu, point to **Programming**.
3. In the submenu, select **Add-in Manager....** The "Add-in Manager" window opens up.
4. In the displayed "Available Add-ins" list, click the name (not the checkbox) of the add-in to be edited, or browse for the required add-in.
5. Click **[Edit]**. The source code is being opened in the VSTA editor for editing.

QUADERA® stores each add-in in a main scripting directory. When required the add-ins are available for all measurement project templates.

NOTE:

For further information on scripting and the programming environment, please refer to the help file for Microsoft Visual Studio Tools for Applications. Use the Help menu of the VSTA editor.

Calling Up the VSTA Help

1. Call up the VSTA editor. (e.g. Edit an available Add-in).
2. In the **Help** menu, select the required item.

or

2. Press the **F1** key.

NOTE:

The VSTA Help includes the help for the specific QUADERA® scripting functionality.

Spectra Library

Spectra Library


A Spectra Library is available for comparison of device spectrum to compound spectra.

The Spectra Library is accessed via the Tools>>Spectra Library menu selection or from any Bargraph Cycles measurement project.

The Spectra Library view and contents can be customized and saved.

Operating the Input/Output Module

- Quadrupole mass spectrometer QMG220: input/output module IO220
- Quadrupole mass spectrometer QMG700: input/output module IO700

⚠ CAUTION	
	<p>Setting digital and analog output values.</p> <p>Improper operation of the input/output module by setting incorrect digital and analog output values can damage the device.</p> <p>Only trained service personnel and personnel with similar training may set the digital and analog output values of the input/output module.</p>

Use the relevant measurement project as a user interface for testing and servicing the input/output module (if existing). For this, connect the device with QUADERA®.

- Digital Inputs: display the states of the digital input (DI) channels:
 - Number: identification of the DI channel,
 - Value: value of the DI channel (On/Off),
- Digital Outputs: switch on and off the digital output channels (DO) manually:
 - Number: identification of the DO channel,
 - Value: value of the DO channel (On/Off),
- Analog Inputs: display the voltage at the analog input (AI):
 - Number: identification of the AI channel,
 - Value: numerical value of the voltage at the AI channel.

Add a measurement task "Add Analog Input Task" to Scan and MID measurement projects to measure the voltage at a analog input.

- Analog Outputs: Change the voltage at the analog output (AO):
 - Number: identification of the analog output,
 - Value: numerical value of the voltage at the analog output.

Creating IO Characteristics

Creating Input/Output Characteristics

Characteristics can be created for Analog Inputs and Outputs. Characteristics can be assigned to one or all devices. Analog I/O Characteristics work with the following devices:

- Quadrupole mass spectrometer QMG220: input/output module IO220
- Quadrupole mass spectrometer QMG700: input/output module IO700

The Characteristics Editor can be accessed from the context-menu of the All Device Status View or from the Device Configuration.

Characteristics can be saved to the software device in QUADERA® from a Measurement Project.

The function of AI/AO Characteristics allows definition of a characteristic set of data that can be applied to an Analog Input or Analog Output. Once defined, these characteristics are then available for use on any Analog Input or Output. For example, a set of data can be defined that produces a charted temperature for an Analog Input.

Example: $X * 1.8 + 32$

The AI/AO Characteristics dialog can be accessed from the Tools >> AI/AO Characteristics menu selection. From this dialog new Characteristics can be created and edited. Characteristics can also be copied (to create a new Characteristic from a standard Characteristic) or deleted. The Characteristic Definition Editor provides a table, graph and formula interface for easy creation of the Characteristic. The Definition Editor is also where the Characteristic type is defined – Analog Input, Analog Output or Analog Input to Analog Output. A name and unit must also be entered in this editor.

The formula interface describes the Y value as a function of X. The formula can use the operators of + - * / ^ as well as the following functions:

Description	Enter as:	Mathematical Equivalent
Calculation of e to the power of X	exn(X)	e^X
Calculation of 10 to the power of X	exp(X)	10^X

QUADERA HTML Help

Calculation of the logarithm, base e	lgn()	ln()
Calculation of the logarithm, base 10	log()	lg()
Squared	sqr()	X^2
Calculation of the square root	srt()	X^(1/2)
Determination of the absolute value	abs()	X
Trigonometric functions	Sin(),Cos(),Tan()	Sin(),Cos(),Tan()
Expressions in parentheses	()	()
Pi	Pi	Pi

The formula parser will indicate when a formula is constructed incorrectly. Note that the parser may indicate 'Operator Input Error' as the formula is being entered. Disregard that message unless it appears when the formula is finalized.

AI/AO Characteristics are then assigned to Analog Inputs and Analog Outputs via the context menu item 'AI/AO Characteristics' in any MID chart. Once a Characteristic is assigned to an Analog Input it is used for that Analog Input in any MID Measurement Project that uses that Analog Input. For example, if Analog Input 1 is wired to a temperature sensor, and a Characteristic is assigned to Analog Input 1, then all MID Measurement Projects that use Analog Input 1 will automatically use that Characteristic.

Warning and Error Messages

List of Events

The event view informs you on the occurred events:

- "Date/Time" displays the time when the event occurred,
- "Source" displays the source that caused the event, e.g. measurement or device,
- "Type" displays the event type ("Information", "Warning", "Error"),
- "Description" displays a brief message text on the event, and specifies warnings and errors. This three-part specification contains:
 - the device specification,
 - the code letter of the event type ("E" means error, "W" means warning),
 - the three-digit identification number of the event.

List of events sorted by identification numbers:

- Warning messages ("W") for the QMG220:
 - W001: "emission current out of tolerance"
 - W002: "emission current wide out of tolerance"
 - W003: "RF-stage temperature is high"
- Error messages ("E") for the QMG220:
 - E001: "external protection triggered"
 - E002: "emission error"
 - E003: "filament 1 defect"
 - E004: "filament 2 defect"
 - E005: "RF-stage switched off because of excessive temperature"
 - E009: "ionsource error"
 - E039: "SEM error"

Warning Messages for the QMG220

Warning Message QMG220.W001

Message text:

"emission current out of tolerance"

Description:

The emission current deviates from the set value.

Message occurs when?

- The emission current deviates 10% and more than 40 μA from the specified value.

Reasons

- The emission current control is faulty,
- The pressure in the recipient is unstable.

Consequences

- Measuring data are corrupt.

Solutions

- Replace the IS220 when the message occurs repeatedly with stable pressure conditions.

Warning Message QMG220.W002**Message text:**

"emission current wide out of tolerance"

Description:

The emission current essentially deviates from the set value.

Message occurs when?

- The emission current deviates more than 20% and more than 40 μA from the specified value.

Reasons

- The emission current control is faulty,
- The pressure in the recipient is unstable.

Consequences

- Measuring data are corrupt.

Solutions

- Replace the IS220 when the message occurs repeatedly with stable pressure conditions.

Warning Message QMG220.W003

Message text:

"RF-stage temperature is high"

Description:

The temperature of the RF stage has exceeded 65°C.

Message occurs when?

- The temperature of the RF stage exceeds 65°C.

Reasons

- Cooling of the RF stage is not sufficient because the fan filter pad is blocked,
- The fan is defective.

Consequences

- Measuring data are corrupt.

Solutions

- Check the fan filter pad,
- Repair the fan.

Error Messages for the QMG220

Error Message QMG220.E001

Message text:

"external protection triggered"

Description:

The protection for SEM and filament has triggered.

Message occurs when?

- The specified threshold is exceeded when monitoring the total pressure,
- The external protection is triggered,
- The total pressure gauge is not properly connected, or the protection input is not properly connected.

Reasons

- Connected total pressure gauge: the pressure has exceeded the specified threshold,
- The total pressure gauge reports an error,
- The total pressure gauge is defective or disconnected,
- The total pressure gauge is switched off.

Consequences

- Filament and SEM are switched on and off depending on the selected protection mode.

Solutions

- Set the protection mode to internal protection.
- Connect a total pressure gauge.
- Modify the threshold of the total pressure gauge.

Error Message QMG220.E002

Message text:

"emission error"

Description:

An emission error occurred.

Message occurs when?

- The specified emission current is not reached,
- The protection current for the filament is triggered.

Reasons

- The filament emission current is too low.

Consequences

- Ionization is impossible,
- Measuring data are not meaningful.

Solutions

- Check the specified protection current for the filament,
- Replace the filament. Refer to the device specific instructions of the QMG (OEM manual) for further information,
- Switch over to the other filament (when existing).

Error Message QMG220.E003**Message text:**

"filament 1 defect"

Description:

The filament 1 is broken.

Message occurs when?

- A broken filament is detected when the device is switched on,
- A broken filament is detected when the filament is switched on,
- The filament is missing.

Reasons

- The filament is defective.

Consequences

- Ionization is impossible,
- The filament can not be switched on,
- Measuring data are not meaningful.

Solutions

- Replace the filament. Refer to the device specific instructions of the QMG (OEM manual) for further information.
- Switch over to the filament 2 (when existing).

Error Message QMG220.E004

Message text:

"filament 2 defect"

Description:

The filament 2 is broken.

Message occurs when?

- A broken filament is detected when the device is switched on,
- A broken filament is detected when the filament is switched on,
- The filament is missing.

Reasons

- The filament is defective.

Consequences

- Ionization is impossible,
- The filament can not be switched on,
- Measuring data are not meaningful.

Solutions

- Replace the filament. Refer to the device specific instructions of the QMG (OEM manual) for further information.
- Switch over to the filament 2 (when existing).

Error Message QMG220.E005**Message text:**

"RF-stage switched off because of excessive temperature"

Description:

The RF stage was switched off because the temperature has exceeded 80°C.

Message occurs when?

- The temperature of the RF stage exceeds 80°C.

Reasons

- Cooling of the RF stage is not sufficient because the fan filter pad is blocked,
- The fan is defective.

Consequences

- The power supply of the RF stage is switched off,
- Measuring data are not meaningful.

Solutions

- Check the fan filter pad,
- Repair the fan,
- Switch the device off, and wait until the RF stage has cooled down. Then switch the device on again.

Error Message QMG220.E009

Message text:

"ionsource error"

Description:

An error occurred in the power supply of the ion source.

Message occurs when?

- The current related to the ion reference voltage is too high,
- The current limit is exceeded in degas mode,
- The power supply of the IS220 is not ok.

Reasons

- The feeder of the IS220 is not ok,
- The connected ion source is short-circuited,
- The specified protection current limit for degas mode is too low.

Consequences

- The ion source is operating faulty,
- Measuring data are not meaningful.

Solutions

- Check and correct contacts and cable of the IS220 power supply,
- Dismount the ion source. Clean or repair it,
- Increase the protection current for degas mode.

Error Message QMG220.E039**Message text:**

"SEM error"

Description:

An error occurred in the control of the SEM voltage.

Message occurs when?

- The SEM voltage deviates 10% and more than 30 V from the specified value,
- In case of a short circuit.

Reasons

- The SEM is contaminated or defective.

Consequences

- The SEM switches off,
- Measuring data are not meaningful when using the SEM.

Solutions

- Check the SEM. Refer to the device specific instructions of the SEM (OEM manual) for further information.

Scripting in QUADERA

NOTE:

You first have to activate the QUADERA® VSTA functionality through an appropriate license key in order to use 'scripting'. Adhere to the notes given in the Release Notes and to the "About..." dialog.

You can use the VSTA functions provided by QUADERA® to automate tasks and to tailor them according to your needs. The available instructions, how to use them, and the syntax is integrated into the Help of the VSTA editor:

- Open the VSTA editor,
- Open the object browser (menu **View** > **Object Browser**),
- Open the library "Quadera",
- Click on the required component,
- The bottom right part of the window displays the available information on the component. Press the **F1** key to invoke the general VSTA Help.

NOTE: QUADERA® provides examples for add-ins and measurement project templates that use these Add-ins. You can use the templates via the start page.

NOTE: VSTA Add-ins can be started from the QUADERA command line if desired. There is a command line option – [/addin] that can be used with the Add-in name. As an example (XP English shown), the following command line can be used to automatically load and start the [GSD320] Add-in:

C:\Program Files\QUADERA\Quadera.exe /addin:GSD320

To modify the command line, create a program shortcut in Windows and edit the shortcut's Properties>>Target field.

Glossary

A

AI: Analog Input: Analog (continuous) input of the mass spectrometer.

amu: atomic mass unit.

Analog Input: Analog (continuous) input of the mass spectrometer.

Analog Output: Analog (continuous) output of the mass spectrometer.

AO: Analog Output: Analog (continuous) output of the mass spectrometer.

B

Background: See Mass spectrometer background.

Bar graph: Display of measuring data on a category axis.

Button: Graphical representation of a binary switch.

C

C-SEM: Secondary electron multiplier with channeltron (also known as channel electron multiplier).

Category: In QUADERA: A non-continuous division of a measuring data axis.

Context menu: A context menu can be called up by clicking certain spots in the graphical user interface with the right mouse button. It contains only menu items that make sense in the clicked area (object specific functions).

D

Data navigator: Operating element for navigation within the measuring data. The data navigator is especially useful when handling large amounts of data.

Degassing: For a specified time, the filament receives a current that is higher than usual. This heats out the measuring head and cleans it from contamination.

DI: Digital Input: Digital (binary) input of the mass spectrometer.

Digital Input: Digital (binary) input of the mass spectrometer.

Digital Output: Digital (binary) output of the mass spectrometer.

Dimension: Relation between a quantity of physics and the basic quantities.

DO: Digital Output: Digital (binary) output of the mass spectrometer.

E

Emission current: Electron current required for ionizing the analysis gas.

Event display: Display for events: Warnings, informations, errors.

F

Filament: Glowing wire which emits the electrons required for ionizing the gas molecules.

FIR: Finite Impulse Response (digital filter).

G

Gas specific calibration factors: Correction factors, used for calculating partial pressures from ion currents.

Graphics: Display with a graphical representation of the measuring values (line graph, bar graph, ...).

GSC: Gas Specific Calibration.

H

Hold: Used if data are being analyzed while a measurement is running. The command freezes the section in its current state (the latest measuring data are not being displayed). However, the measurement continues in the background.

I

Ion source optimization: Calibration process during which the ion source is adjusted in order to optimize the ion current with respect to the intensity and/or the peak shape.

M

Mass scale calibration: Correction between nominal mass number and actual peak maximum.

Mass spectrometer background: Background determination by the software. Mostly, a zero gas is used for this.

MCD: Multiple Concentration Determination. In this measuring mode, the concentration of the individual gas components is calculated from measured ion currents.

Measurement project: Contains all instruments required to perform a specific measurement task. One device is assigned to each measurement project. It is possible that several measurement projects relate to the same device.

Measurement project template: See Template.

Measurement task: Constitutes the basic component of a recipe and contains the measuring mode and all parameters required to specify this mode. Measurement tasks can be configured.

Measuring mode: The different types of measurement that are supported by the device.

MID: Multiple Ion Detection. In this measuring mode, the intensity for specified masses is measured as a partial pressure or ion current.

MS: Mass spectrometer.

N

Nominal mass: Expected mass of an element.

O

Object: General term for elements that are being used in the software in any way, e.g. chart, task.

Offset: Offset of a real measuring amplifier from zero.

P

Parameter set: Group of parameters that are related or belong together otherwise (settings).

Partial pressure: Pressure that is being created by an individual component in a gas mixture.

Peak: A scan-analog spectrum consists of a number of peaks. These represent fractions of the individual gas components at the respective masses.

PGA: Process gas analysis.

ppb: Parts per billion (1 : 1,000,000,000).

ppm: Parts per million (1 : 1,000,000).

Process gas analysis: Analysis of gas mixtures that are being expected in a process.

Property dialog field: Dialog window, generally containing several tabs.

Q

QC: Quadrupole Controller. See operating instructions QMG.

QMG220: High-end mass spectrometer.

QMG700: High-end mass spectrometer.

QUADERA: Operation and analysis software for the QMG mass spectrometers.

R

Recipe: A recipe is a sequence of measurement tasks.

RF: Radio Frequency.

RGA: Residual Gas Analyzer.

S

Scan: See Scan Analog.

Scan Analog: Ion current as a function of m/e.

Scan speed: Sampling rate for scan-analog measurements. In most cases the time/mass.

Scan-F filter: FIR filter, used for smoothing a scan-analog signal.

Scripting: Programming of specific routines. In QUADERA, scripting has been implemented with VSTA.

Section: Part of the working area. Any working area can be divided into so-called sections by the user. Each section can be filled with a graphical object (e.g. measuring data display).

SEM: Secondary Electron Multiplier.

Sensitivity: The sensitivity is the basis to calculate partial pressures from ion currents. The sensitivity is used together with the gas specific calibration factors, and can be determined from measurements.

SEV: Sekundärelektronenvervielfacher (German expression for SEM).

SPM: Sputter Process Monitor.

T

Template: Predefined settings which help the user to create a measurement project (configuration of the measurement without measuring data).

Toolbox: Graphical operating element which depicts functions with small pictograms. The functions are activated or executed by dragging & dropping the related pictograms.

Trend: Course of a value with time.

Trend display: Graphical display for the course of a measured quantity with time.

Tune Mode: Procedure for tuning a device such as the ion source and optimizing the signal shape.

U

Unit: Quantity of physics = Numerical value * unit.

V

VBA: Visual Basic for Applications. Scripting language by Microsoft which is used for programming in applications. Followed by VSTA.

VSTA: Visual Studio Tools for Applications. Development system to customize applications by using the .NET framework. Replaces VBA.

W

Working area: Part of the measurement project window or recipe. The working area is used to display measuring data or to specify parameters for the currently selected recipe.

Workspace: See Working area

WYSIWYG: "What You See Is What You Get": The displayed screen is being output at the printer as faithfully as possible.

Index

A

About.....	23	Manager	199, 201
Active Set	113	AI Channel.....	172, 177
Actual Mass.....	132	Amplifier offset	135
Add Analog Input Editor	50	Analog filter	172, 177
Add Analog Input Task.....	50	Analog input editor.....	205
Add Analog Output Editor	50	Analog Inputs	206
Add Chart Element	50	Analog output editor.....	205
Add Digital Input Editor.....	50	Analog Signal Filter	172, 177
Add Digital Output Editor	50	Analyser Detector Type.....	28
Add MCD Chart.....	50	Analysis matrix.....	181
Add MCD Task	50	AO Channel.....	172, 177
Add MID Chart.....	50	AO Mode.....	172
Add MID Task.....	50	AO Range	172
Add Peak Task.....	50	Apply to Background Library.....	146
Add Scan Chart.....	50	Apply to MCD Calibration Factor Library.....	155
Add Scan Task.....	50	Arrange Icons.....	101
Add Total Pressure Task.....	50	Auto Hide.....	70
Add Working Area	50, 98	Automating	194
Add-in	195	Autorange Mode.....	172, 177
Activating.....	199	Available Add-ins	199, 201
Copying	196	Average.....	188
Creating.....	198	Axial	113
Deleting	197	Axis X	66
Editing.....	201	Axis Y.....	66
		Axis Y1	66

QUADERA HTML Help

Axis Y2	66	Calling up context menus	60, 61
B		Capturing screens	71
Background.....	143, 144	Cascade.....	101
Background library	144, 146	Cathode.....	113
Bar	66, 84	Channel.....	35, 48
C		Channel parameter editor.....	170
Calibration	73, 109	Characteristics.....	206
Calibration and Tuning.....	73	Characteristics Editor.....	206
Calibration factor	150, 157	Chart display.....	77, 82, 84
Calibration factor library.....	157	Chart element	35
Calibration gas	149	Checkbox.....	38
Calibration project.....	73, 109	Click.....	40
Background	143, 144	Close.....	62, 86, 90
Calibration factor.....	150, 157	Close All Windows	101
File location.....	91	Closing	
Gas specific calibration.....	149, 150	Application	62
Ion source.....	110, 111	Measurement project	90
Mass scale.....	124, 126, 128	Quadera.....	86
Offset	134, 135	Window	62, 101
RF tuning	139	Color	66, 94
Calibration recipe	181	Common SEM voltage.....	57, 172, 177
Calling up		Communication Settings	104
Context menu.....	61	Component	152, 155
Help	20	Concentration.....	152
Macro	200	Configuration.....	1, 27
VSTA editor	202	Configuration project	73, 109
VSTA help	203, 219	Connect.....	57, 107

- Contents.....20
- Context menu..... 60, 61
- Chart..... 66, 140
- Frame of the section.....65
- GSC matrix editor 153
- Mass Scale Tune Fine Editor..... 132
- Menu bar63
- Recipe editor 171
- Recipe selection64
- Title bar62
- Window title70
- Copy Parameter To All 170
- Copyright..... 7
- CP-Level 172, 177
- Create Add-in 198
- Crossbeam..... 28, 113, 117
- Cross-references..... 9
- Cursor77
- Curve color94
- Customize.....63
- D**
- Data files91
- Data navigator.....65, 77, 79
- Delete Background Library 146
- Delete Mass Scale Tune Fine Entries
..... 132
- Delete MCD Calibration Factor Library
..... 157
- Delete Offset Entries..... 137
- Delete section..... 50, 97
- Delete selected Component ...152, 170
- Delete selected Mass 152
- Delete selected rows..... 132
- Delete working area99
- Detector Range..... 137, 172, 177
- Detector Type..... 172, 177, 182
- Device35
- Device parameter..... 28, 57
- Device Sensitivity..... 159
- Device setting28
- Device status..... 57, 103
- Device status view 57, 58, 103
- Device Status View allows58
- Device Status View shows58
- Digital input editor 205
- Digital output editor 205
- Directories 17, 91
- Disconnect 57, 106
- Display 66, 95
- DO# A..... 172, 177, 182
- DO# B..... 172, 177, 182
- Dockable70
- Docker window 70, 103
- Double-click40
- Drag&Drop.....40

QUADERA HTML Help

Dropdown list38

Dwell172, 177, 182

E

Editing add-ins 201

Editing macros..... 201

Editing parameters..... 170

Editor

 Analog input/output..... 205

 Digital input/output 205

 GSC matrix 152

 Ion source..... 113

 Mass Scale Tune Coarse 130

 Mass Scale Tune Fine 132

 MCD matrix 181

 MCD recipe..... 181

 Recipe 170

 VSTA..... 202

Electrometer preamplifier 137

Emission current 113

Error24

Error message 208

Event view 59, 103

Events..... 208

Exit.....86

Exiting QUADERA86

Export89

EXT IN50

Extraction 113

F

Factor 155

Faraday 28, 137, 146

Field axis 113

Filament number..... 113

Filament protection current 113

Filament, switch on/off 57, 105

File extension 161

File location.....91

FirstMass 172

Floating70

Focus 113

Freezing the display 100

G

Gain.....172, 177

Gas specific calibration..... 149

 GSC matrix editor..... 152

 GSC result view 155

 Parameter 155

Grid 28, 113, 118

GSC result view 155

H

Hardware.....19

Help.....46

 Calling up.....20

 Display21

Printing.....	22		
VSTA.....	203		
Hide.....	70, 103		
High sensitivity.....	28, 113, 120, 121		
Hold Off.....	66, 79, 100		
Hold On.....	66, 79, 100		
I			
Index.....	20		
Inner deflection.....	113		
Input/output module.....	205		
Installation.....	25, 26		
Intensity.....	146, 155		
Internal standard.....	152, 157		
IO220.....	28, 205		
IO700.....	205		
Ion counter.....	146		
Ion reference.....	113		
Ion source.....	28		
Optimizing.....	111, 117, 118, 119, 120, 121		
Parameter.....	113		
Tuning.....	110, 111		
Ion source type.....	28, 113		
Ion source voltages.....	113, 117, 118, 119, 120, 121		
IP address.....	104		
K			
Keyboard shortcut.....	41, 42		
L			
Legend.....	66		
Level A.....	172, 177, 182		
Level B.....	172, 177, 182		
License agreement.....	3		
License key.....	23, 26		
Line thickness.....	95		
Lock the Toolbars.....	63		
M			
Macro.....	194		
Creating.....	198		
Editing.....	201		
Running.....	200		
Macros.....	45		
Manuals.....	9		
Marker.....	66		
Mass.....	146, 152, 155, 177		
Mass Range.....	28		
Mass resolution.....	172		
Mass scale.....	124		
Coarse tuning.....	126, 130		
Fine tuning.....	128, 132		
Parameters.....	130, 132		
Mass Scale Adjust.....	128		
Mass Scale Offset.....	130		
Mass Scale Slope.....	130		
Mass spectrometer.....	35		

QUADERA HTML Help

MassMode	172	Measurement task.....	35, 48
Maximize	62	Add	48, 170
Maximum.....	189	Delete	48, 170
MCD calibration factor library.....	157	MCD	84, 164
MCD measurement project	164, 181	MID.....	76, 84
Measurement	35, 161	Name	177
Measurement parameter file ...	73, 161	Recipe	35, 55, 168
Measurement project.....	35, 161	Scan.....	75, 82
Closing	90	Sequence.....	170
Exporting	89, 91	Total pressure.....	166
File location.....	91	Measuring data.....	55
MCD	164	Average	188
MID.....	163	Closing	90
Open	73, 87	Displaying	66, 92
Recipe	170	Exporting	89
Saving	90	Maximum.....	189
Scan.....	162	Minimum.....	187
Starting	105	Opening	73, 87
Stopping	105	Saving	90
Template	73, 161	Standard deviation	190
Window	53	Measuring mode	107
Measurement project template	73, 161	Measuring range	172, 177
Create	167	Menu bar	45, 63
File location.....	91	Menu commands.....	45
Open	73	Menus	45
Select.....	73	MID measurement project.....	163
Measurement project window	53	Minimize	62

Minimize all windows	101	Help topic.....	22
Minimum	187	Screenshot	71
Move.....	62	Product description.....	15
Multiplexing	47	Programming.....	198, 199, 200, 201
Multisensor	27, 47	Project	35, 161
N		Protection	28
Network settings.....	1	Q	
New section	96	QC	177
New working area	98	QMP.....	161
Nominal Mass	132	QMT.....	161
O		Quadera	15
Object	35	Exiting	86
Offset.....	130, 134	Installing.....	25, 26
Determining	135	License key	26
Parameter	137	Main features.....	16
Offset Mass.....	137	Migrating from Quadstar.....	11
Open.....	87	Product description.....	15
Operating voltage	57, 177	Release Notes	1
Options	47, 91	Scope of delivery.....	17
Outer deflection.....	113	Screenshot	71
P		Setting up	27
Parameter	113, 130, 132, 137, 146, 152, 170, 172, 177, 181, 182	Start page.....	73
Partial Pressure	159, 160	Starting	72
Pause Calibrate.....	172, 177	Uninstalling	34
Pressure gauge.....	28	Update	32, 33
Printing		Upgrade.....	32, 33
		User interface	37

QUADERA HTML Help

Version	23	RF-Polarity	113
VSTA reference	219	Run.....	105, 200
Quadrupole controller	177	Running macros	200
Quadstar	11, 12, 13		
R		S	
Radio button	38	Save	90
Range Limit.....	172, 177	Save As Template	167
Recent files	88	Scan measurement project	162
Recipe	35, 55, 168	Scope of delivery	17
Parameters 113, 130, 132, 137, 146,		Screen elements	38
152, 170, 172, 177, 181, 182		Screenshots	71
Selection.....	54	Scripting.....	194, 195, 219
Recipe editor	170	Section	35, 55
Recipe parameter. 113, 130, 132, 137,		Add.....	50, 96
146, 152, 170, 172, 177, 181, 182		Adjust.....	92
Release Notes.....	1	Chart.....	77
Remove Chart Element	50	Delete	48, 50, 97
Remove Section.....	50, 97	Recipe editor	170
Remove Section Content	50	Remove	48, 50, 97
Remove Working Area	50, 99	Split	48, 50, 96
Rename selected tab	64, 65	SEM	28, 57, 137, 146, 172, 177
Report an error.....	24	SEM Voltage.....	57, 172, 177
Reset Arrows.....	140	SEM, switch on/off	57, 105
Reset zoom.....	66, 93	Sensitivity.....	159, 160
Resolution.....	172, 177	Sensitivity Determination	160
Restore	62	Set as internal standard	152
RF generator	140, 142	Setting up.....	27
RF tuning.....	140, 142	SETUP	25

Shortcut	41, 42	State.....	172, 177, 182
Assign	42	Status view	57
Change.....	42	Stop.....	105
Delete	42	Stopping the measurement	57, 105
Show navigator	65	System information	23
Show Start Page	73	System requirements	19
Simulation mode.....	28, 107, 108	T	
Size	62	Table.....	66, 84
Slope	130	Task.....	35, 48
Smooth Chart Lines.....	95	Task Name.....	172, 177, 182
Software.....	19	Template	73, 161
Software device	35	Terminology	12
SpecNeg	113	Tile Horizontally	101
SpecPos.....	113	Tile Vertically.....	101
Spectra Library.....	204	Title bar.....	44
Speed	172	Tool	48, 204
Spin button.....	38	Applying	49
Split Section Bottom.....	50	Overview	50
Split Section Left.....	50	Toolbox	35, 48, 50, 103
Split Section Right.....	50	Tooltip.....	38
Split Section Top.....	50	Total pressure	28, 166
SPM	28, 113, 119	Total Pressure Measurement.....	166
Standard deviation.....	190	TP RS 485 Address.....	28
Standard directories	17	TP Status.....	28
Start mass	172	TP Type	28
Start page	73	Trend	66, 84
Starting the measurement.....	57, 105	Trip function.....	177, 184, 186

QUADERA HTML Help

Trip Type 172, 177, 182, 184, 186

Tuning

Ion source..... 110

Mass scale.....124, 126, 128

Tuning voltage..... 140, 142

U

Update25, 32, 33

Upgrade25, 32, 33

User interface..... 37, 38

V

VBA 194

Version number23, 32, 33

Visual Studio Tools for Applications
.....194, 202, 203

VSTA.....194, 202, 203

VSTA reference.....219

W

Warning message208

Wehnelt..... 113

Width..... 172

Window 103

Arrange 102

Close..... 62, 101

Displaying 101

Dockable.....70

Floating70

Hide 70, 103

Show..... 70, 103

Switch 101

Window size62

Working area..... 35, 55

Create 50, 98

Delete 50, 99

Rename 64, 65

Split 50, 96

Working area selection.....56

X

X-axis66

Y

Y-axis.....66

Z

Zero gas143, 144

Zero gas library144, 146

Zoom Out66

Zoom Range.....93

Zooming 81, 93